


Data Path : Z:\HPCHEM1\BNA_F\Data\BF012717\
 Data File : BF092581.D
 Acq On : 27 Jan 2017 17:36
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF012417.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jan 24 13:48:07 2017

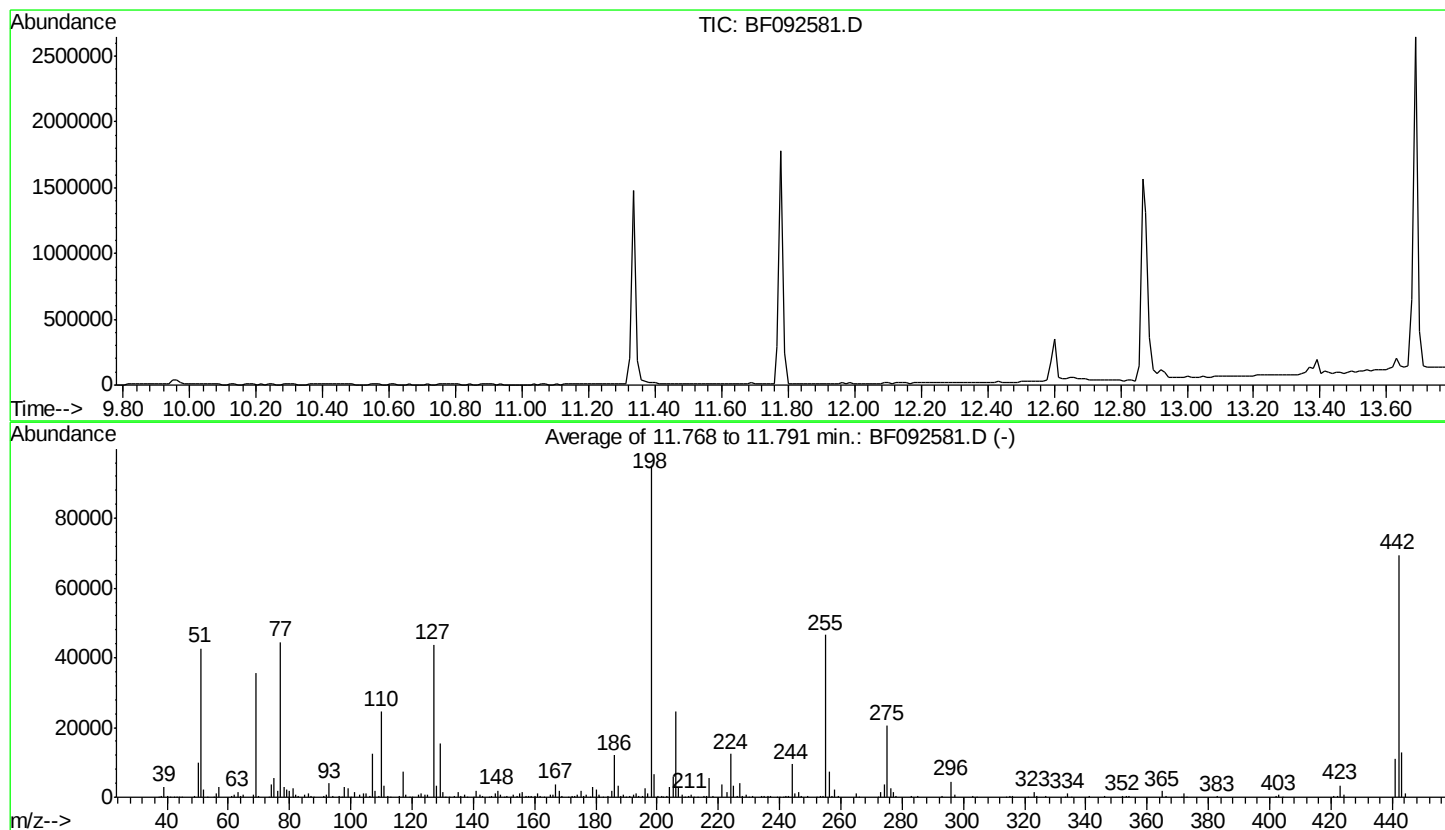

AutoFind: Scans 847, 848, 849; Background Corrected with Scan 844

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.8	42601	PASS
68	69	0.00	2	1.8	652	PASS
69	198	0.00	100	37.4	35577	PASS
70	69	0.00	2	0.6	212	PASS
127	198	10	80	46.0	43706	PASS
197	198	0.00	2	1.1	1012	PASS
198	198	100	100	100.0	95109	PASS
199	198	5	9	6.9	6548	PASS
275	198	10	60	21.6	20560	PASS
365	198	1	100	1.9	1788	PASS
441	442	0.01	24	16.1	11210	PASS
442	198	50	100	73.1	69540	PASS
443	442	15	24	18.5	12855	PASS