


Data Path : Z:\HPCHEM1\BNA_F\Data\BF012717\
 Data File : BF092606.D
 Acq On : 28 Jan 2017 5:39
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF012417.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jan 24 13:48:07 2017

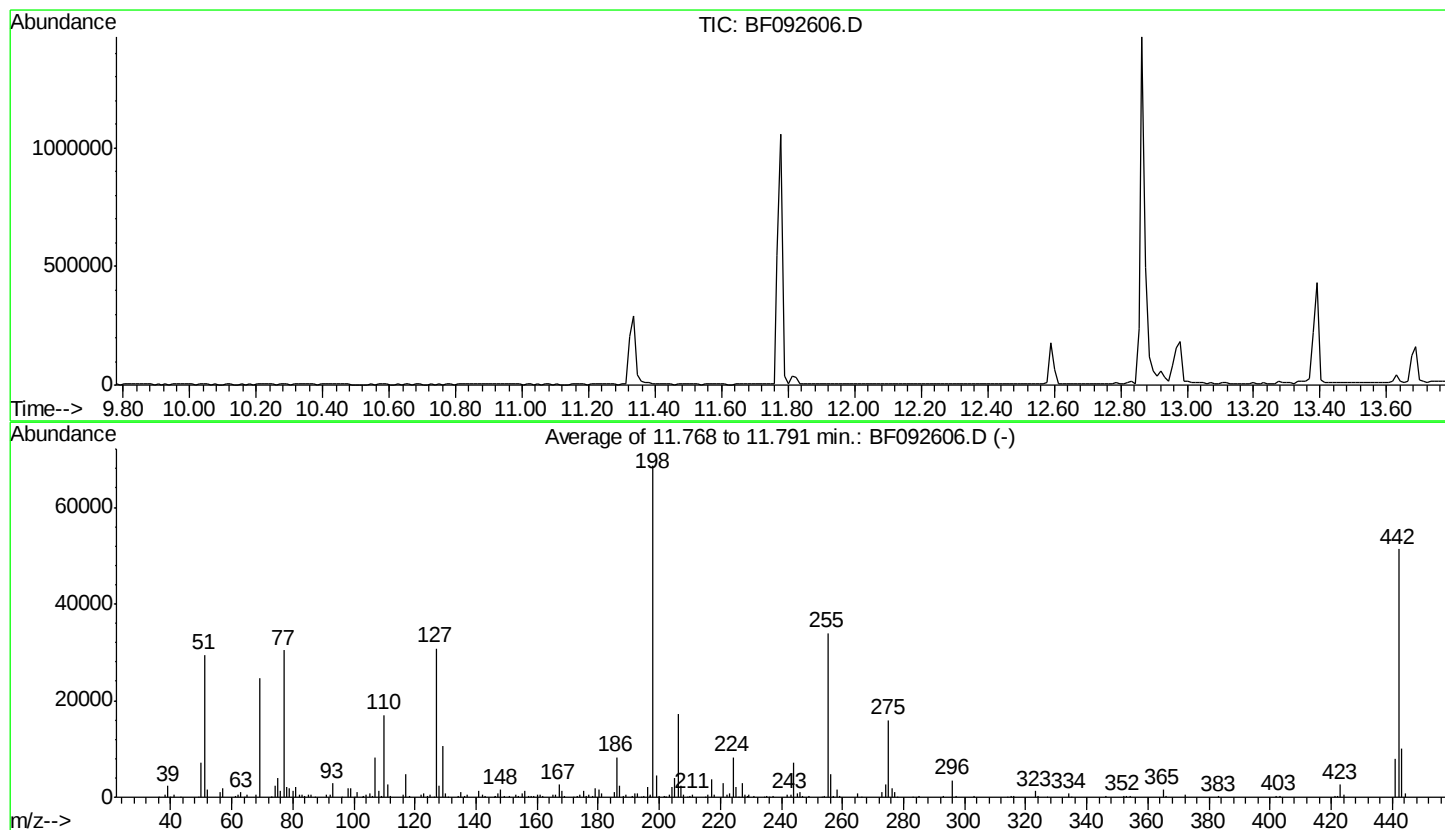

AutoFind: Scans 847, 848, 849; Background Corrected with Scan 843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.0	29491	PASS
68	69	0.00	2	1.9	455	PASS
69	198	0.00	100	35.8	24551	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	44.8	30747	PASS
197	198	0.00	2	0.8	569	PASS
198	198	100	100	100.0	68618	PASS
199	198	5	9	6.8	4635	PASS
275	198	10	60	23.4	16025	PASS
365	198	1	100	2.2	1502	PASS
441	442	0.01	24	15.5	7948	PASS
442	198	50	100	74.8	51323	PASS
443	442	15	24	19.5	9992	PASS