
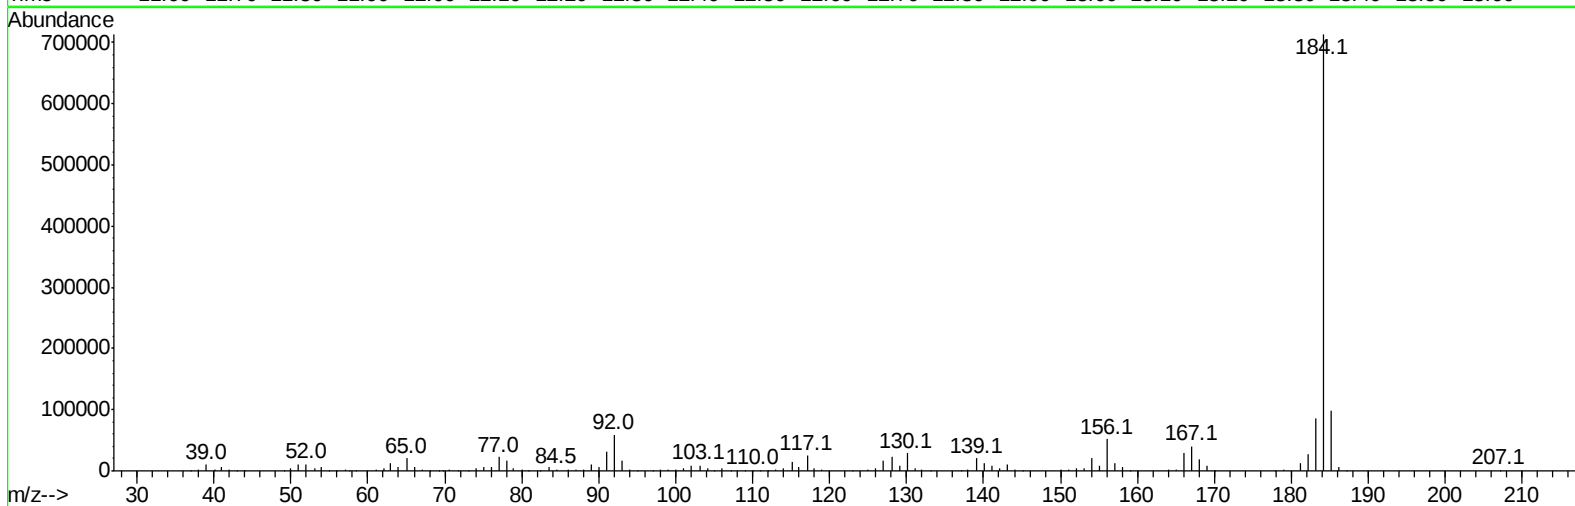


Data Path : U:\HPCHEM1\BNA F\DATA\BF012718\
Data File : BF102498.D
Acq On : 27 Jan 2018 9:09
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 29 02:12:58 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF012218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jan 27 20:48:40 2018
Response via : Initial Calibration

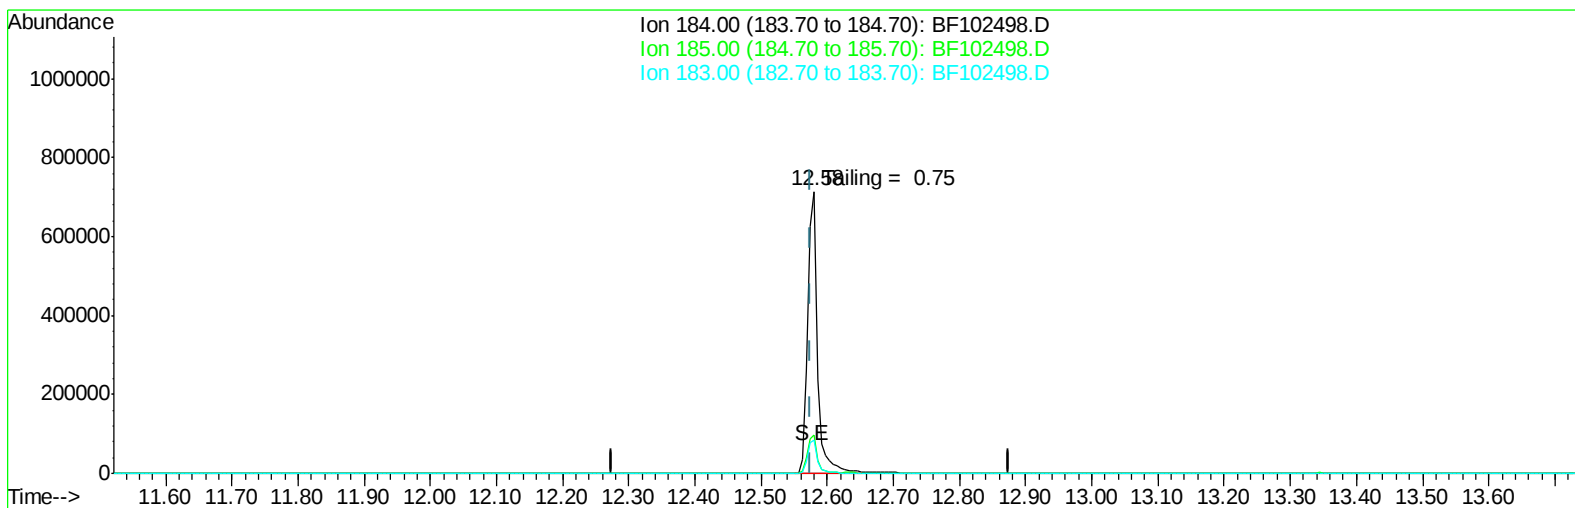

TIC: BF102498.D

(76) Benzidine



12.580min (+0.006) 0.00ng

response 758138

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	13.72
183.00	11.60	12.00
0.00	0.00	0.00

Data Path : U:\HPCHEM1\BNA F\DATA\BF012718\
Data File : BF102498.D
Acq On : 27 Jan 2018 9:09
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 29 02:12:58 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF012218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jan 27 20:48:40 2018
Response via : Initial Calibration

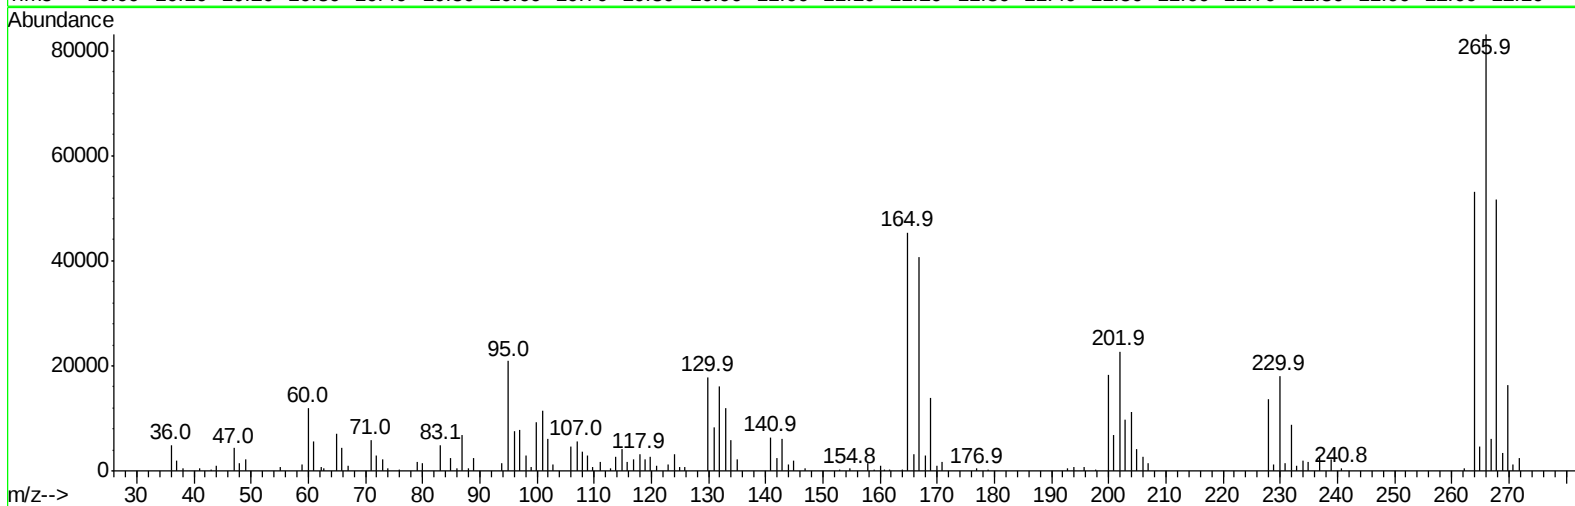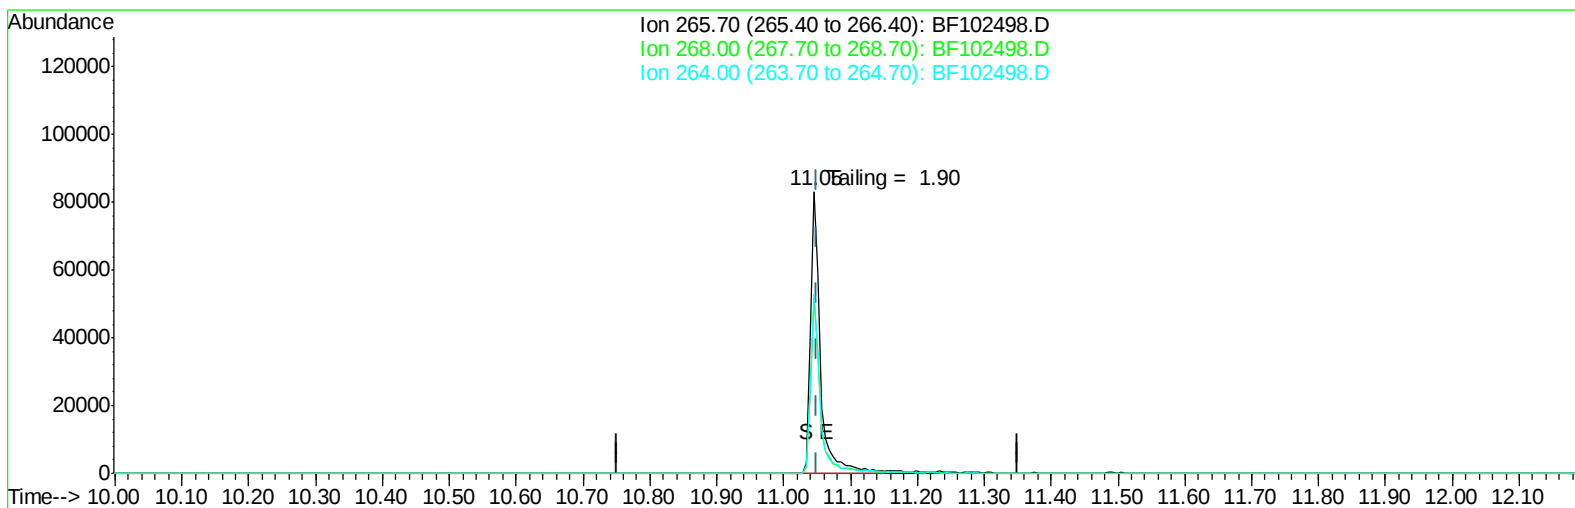

TIC: BF102498.D

(69) Pentachlorophenol (C)

11.045min (-0.006) 44822.29ng

response 89012

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	62.25
264.00	61.90	63.84
0.00	0.00	0.00