
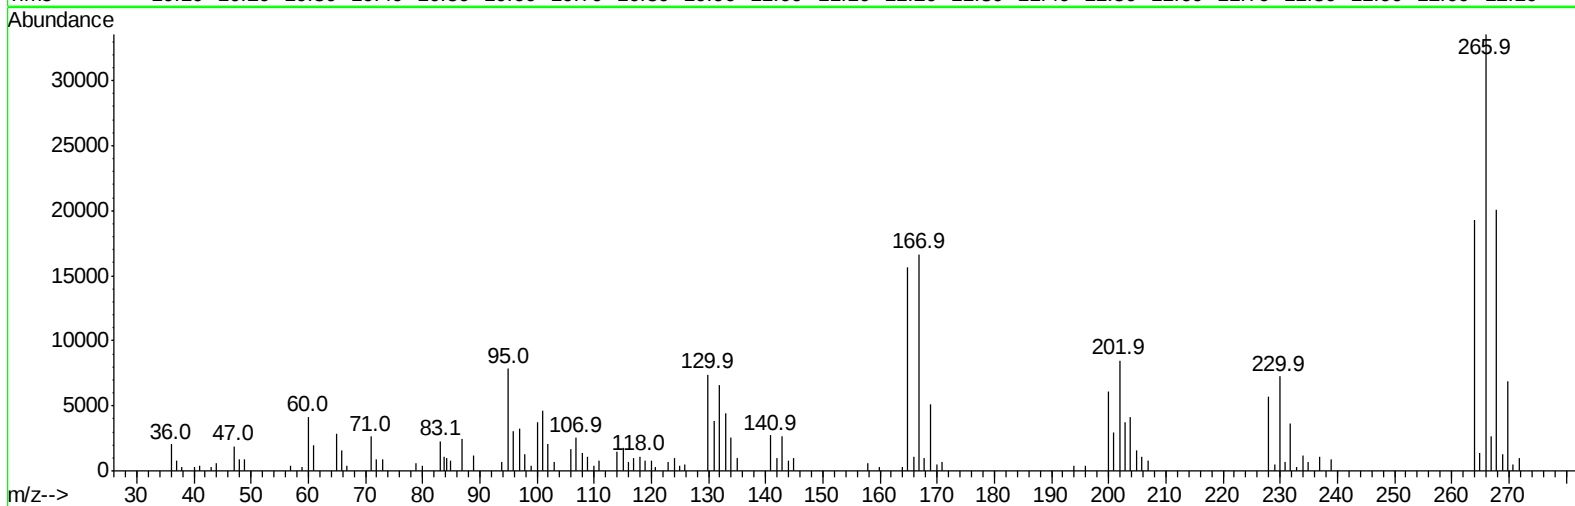


Data Path : U:\HPCHEM1\BNA F\DATA\BF012718\
Data File : BF102539.D
Acq On : 28 Jan 2018 5:14
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 29 02:17:14 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF012218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jan 27 20:48:40 2018
Response via : Initial Calibration

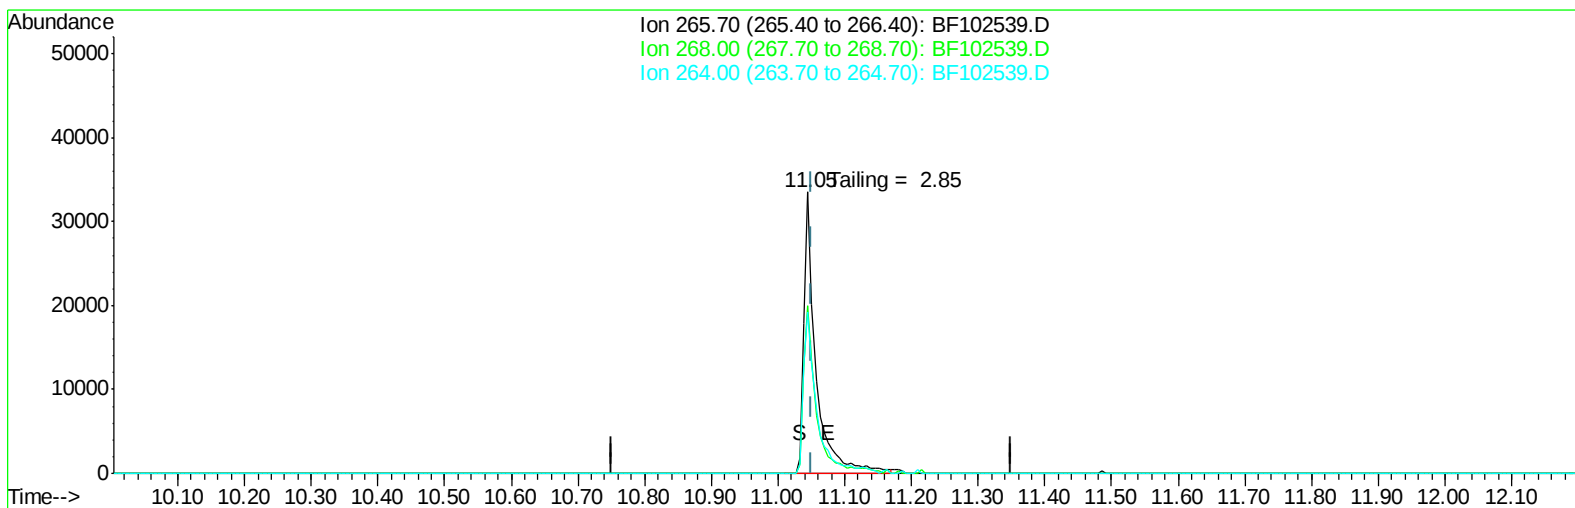

TIC: BF102539.D

(69) Pentachlorophenol (C)



11.045min (-0.006) 37922.34ng

response 41732

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	59.73
264.00	61.90	57.34
0.00	0.00	0.00

Data Path : U:\HPCHEM1\BNA F\DATA\BF012718\
Data File : BF102539.D
Acq On : 28 Jan 2018 5:14
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 29 02:17:14 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF012218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jan 27 20:48:40 2018
Response via : Initial Calibration

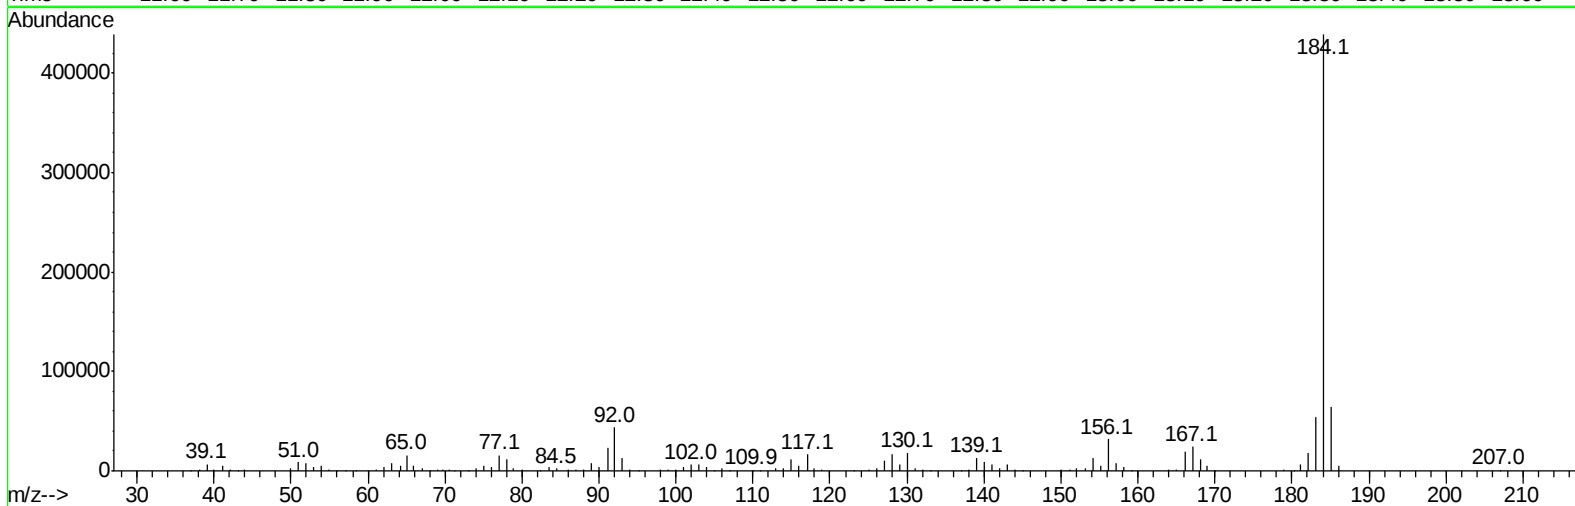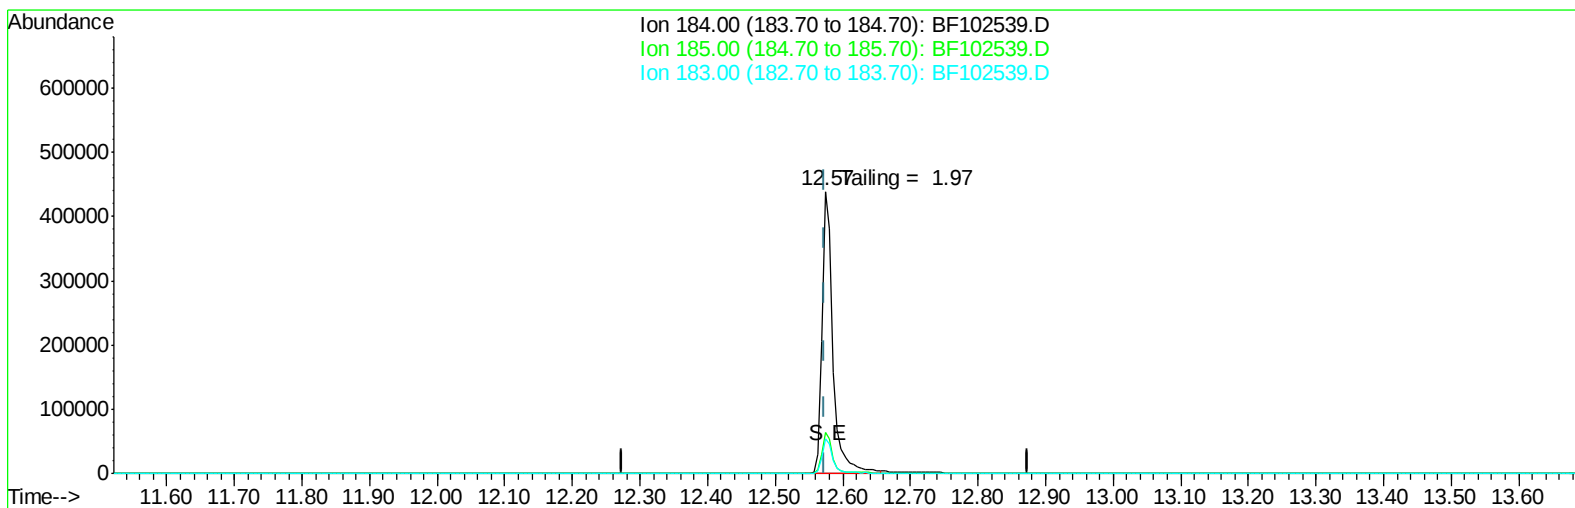

TIC: BF102539.D

(76) Benzidine

12.574min (-0.000) 0.00ng

response 505842

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.57
183.00	11.60	12.34
0.00	0.00	0.00