


Data Path : Z:\HPCHEM1\BNA_F\Data\BF012718\
 Data File : BF102498.D
 Acq On : 27 Jan 2018 9:09
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF012218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Jan 27 20:48:40 2018

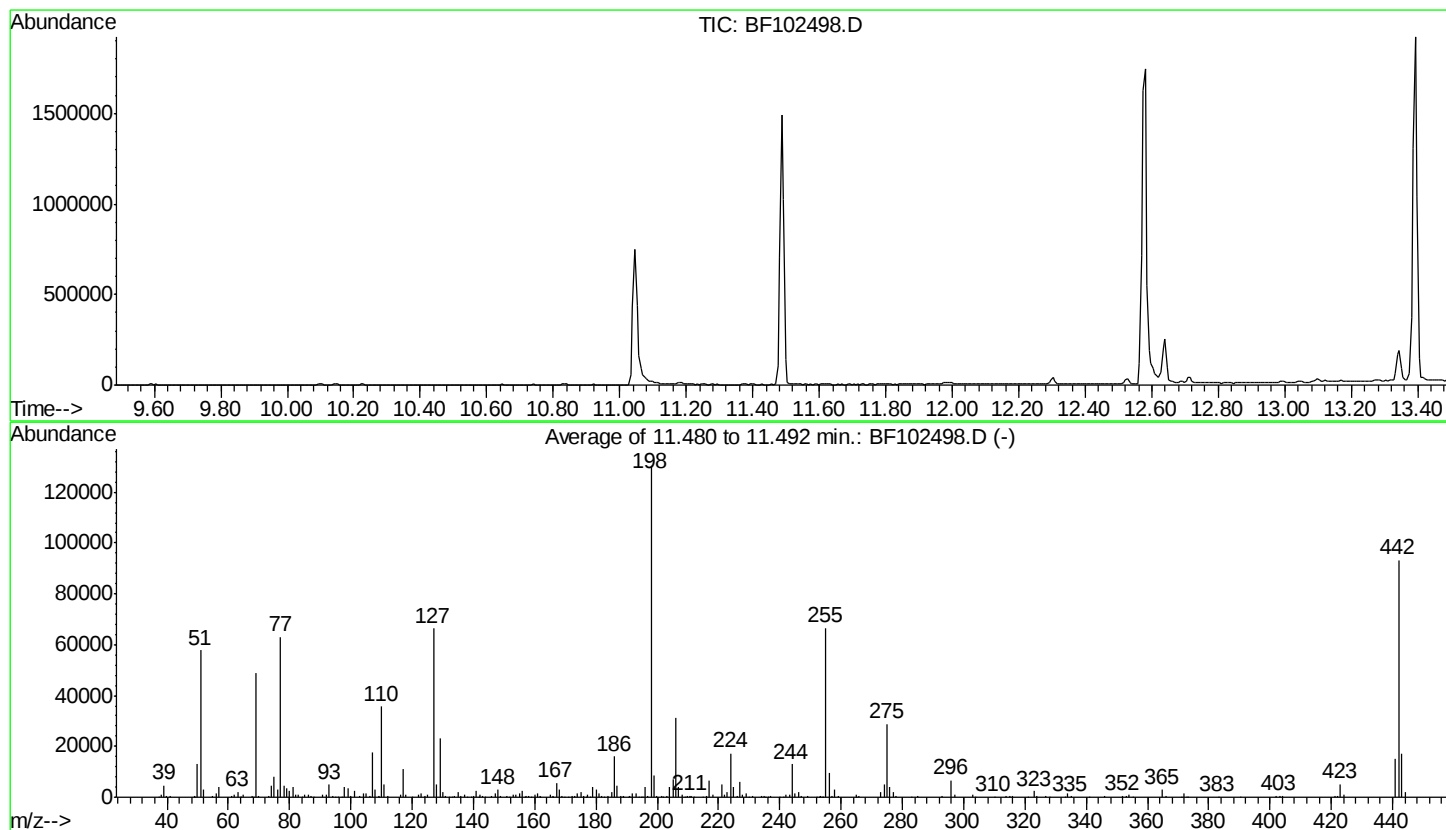

AutoFind: Scans 1597, 1598, 1599; Background Corrected with Scan 1592

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.3	57821	PASS
68	69	0.00	2	1.4	701	PASS
69	198	0.00	100	37.3	48628	PASS
70	69	0.00	2	0.6	289	PASS
127	198	10	80	50.9	66362	PASS
197	198	0.00	2	0.3	411	PASS
198	198	100	100	100.0	130445	PASS
199	198	5	9	6.6	8634	PASS
275	198	10	60	22.2	28956	PASS
365	198	1	100	2.3	2968	PASS
441	443	0.01	100	86.6	15013	PASS
442	198	50	100	71.5	93205	PASS
443	442	15	24	18.6	17345	PASS