


Data Path : Z:\HPCHEM1\BNA_F\Data\BF012718\
 Data File : BF102512.D
 Acq On : 27 Jan 2018 16:05
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF012218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Jan 27 20:48:40 2018

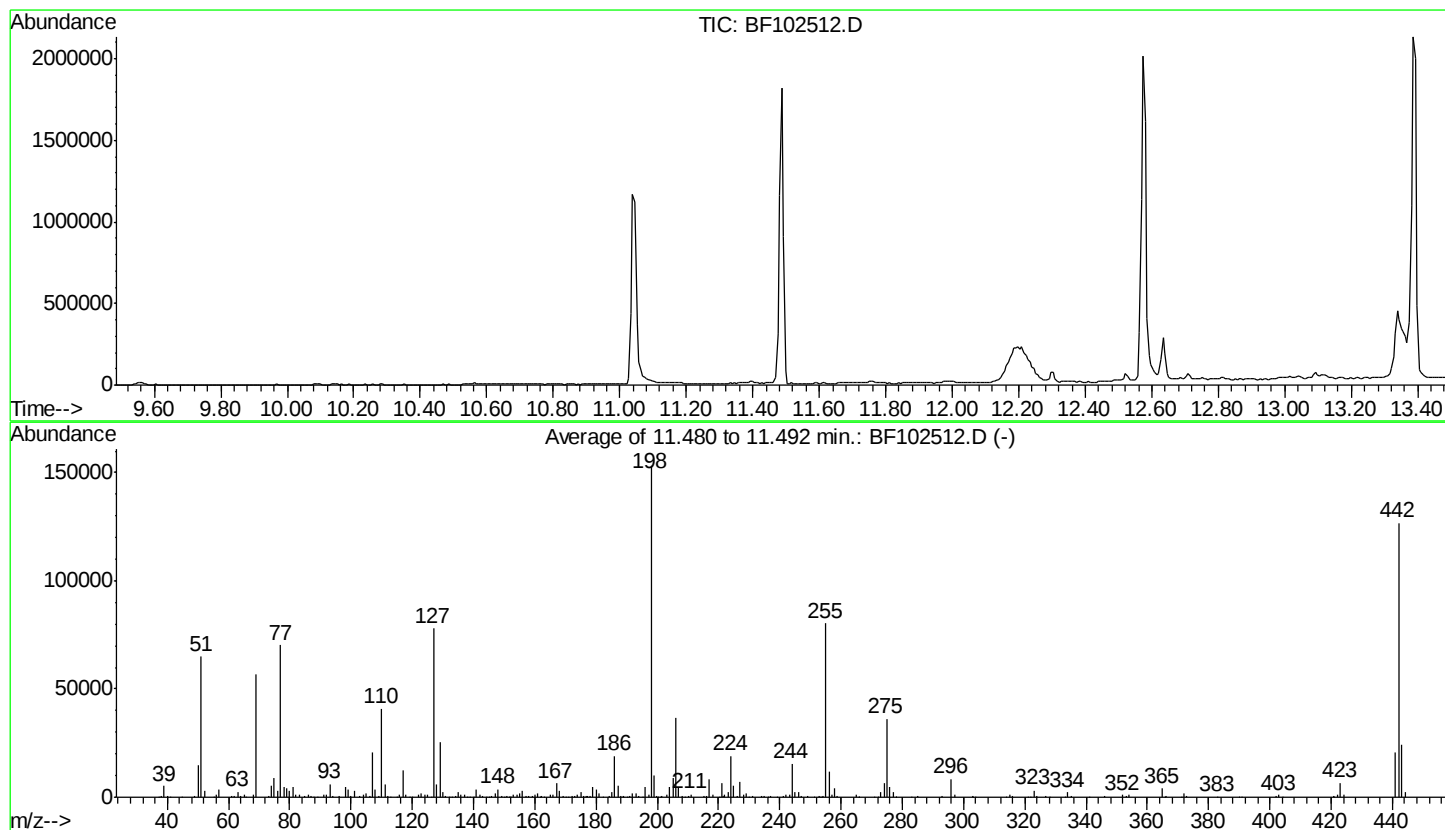

AutoFind: Scans 1597, 1598, 1599; Background Corrected with Scan 1592

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.4	64901	PASS
68	69	0.00	2	1.9	1068	PASS
69	198	0.00	100	36.9	56513	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	50.9	77994	PASS
197	198	0.00	2	0.7	1124	PASS
198	198	100	100	100.0	153224	PASS
199	198	5	9	6.4	9791	PASS
275	198	10	60	23.6	36101	PASS
365	198	1	100	2.7	4091	PASS
441	443	0.01	100	85.0	20518	PASS
442	198	50	100	82.8	126832	PASS
443	442	15	24	19.0	24130	PASS