


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF012720\
 Data File : BF118713.D
 Acq On : 27 Jan 2020 11:44
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jan 27 14:24:10 2020

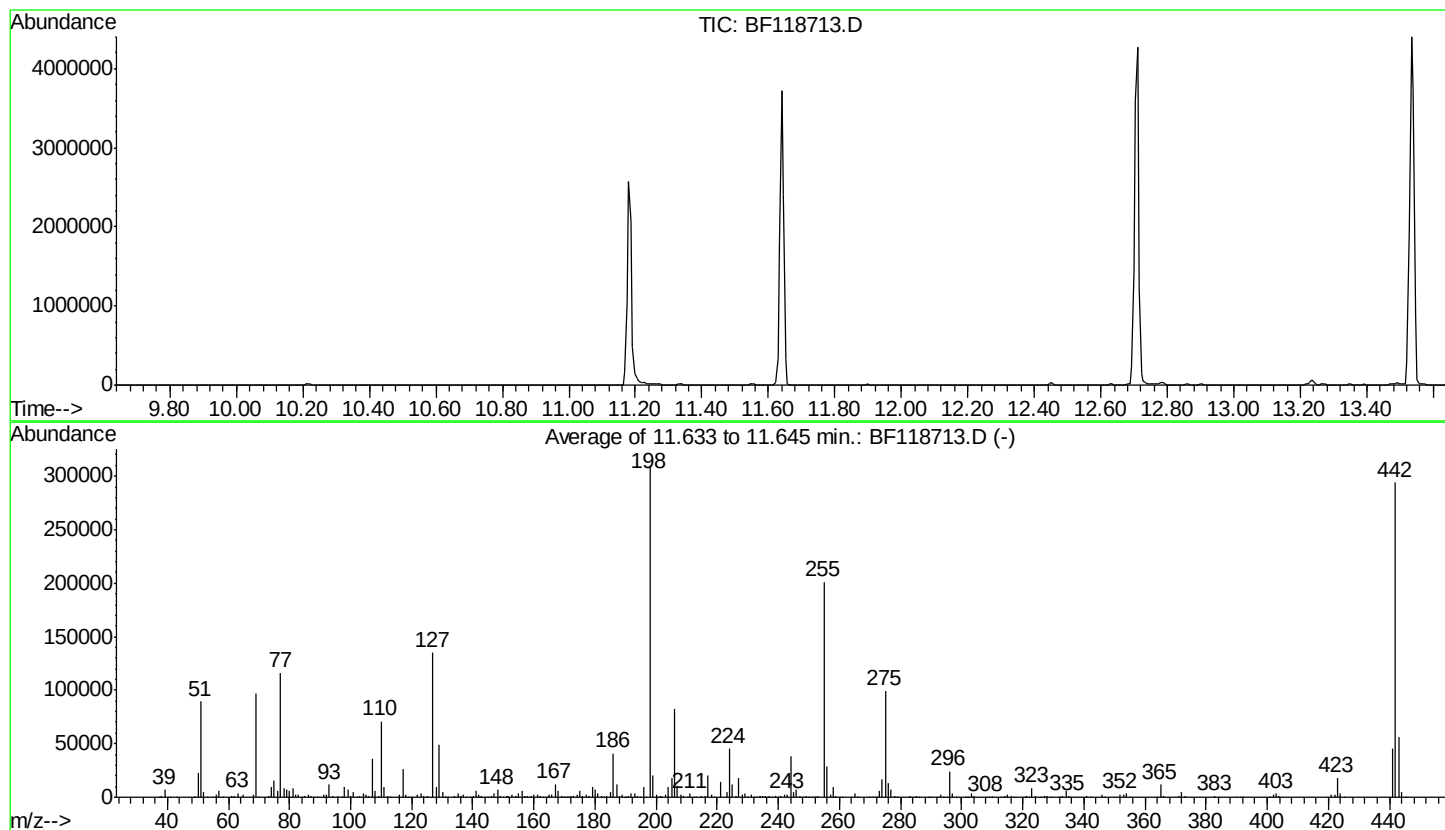

AutoFind: Scans 1623, 1624, 1625; Background Corrected with Scan 1618

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.8	89136	PASS
68	69	0.00	2	1.9	1882	PASS
69	198	0.00	100	31.4	97168	PASS
70	69	0.00	2	0.6	545	PASS
127	198	10	80	43.6	135005	PASS
197	198	0.00	2	0.2	559	PASS
198	198	100	100	100.0	309802	PASS
199	198	5	9	6.7	20837	PASS
275	198	10	60	32.1	99429	PASS
365	198	1	100	3.9	11956	PASS
441	198	0.01	100	14.7	45568	PASS
442	198	50	100	94.8	293840	PASS
443	442	15	24	19.2	56490	PASS