


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012722\
 Data File : BF126704.D
 Acq On : 27 Jan 2022 09:50
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011822.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jan 27 03:09:40 2022

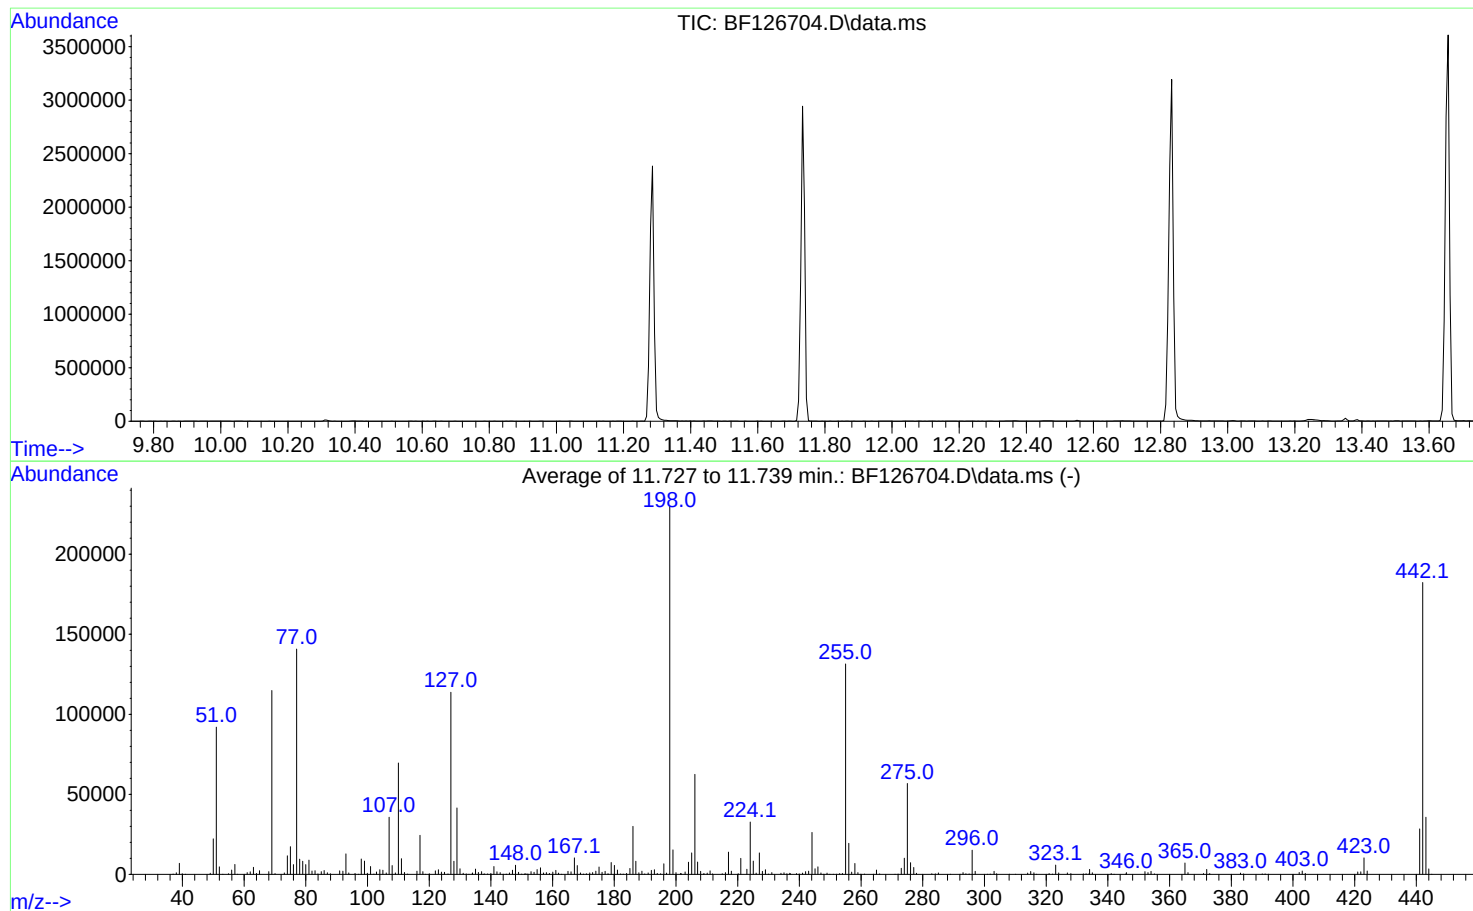




AutoFind: Scans 1639, 1640, 1641; Background Corrected with Scan 1634

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.0	91944	PASS
68	69	0.00	2	1.5	1732	PASS
69	198	0.00	100	50.0	114832	PASS
70	69	0.00	2	0.4	498	PASS
127	198	10	80	49.5	113787	PASS
197	198	0.00	2	0.4	833	PASS
198	198	100	100	100.0	229824	PASS
199	198	5	9	6.7	15291	PASS
275	198	10	60	24.7	56768	PASS
365	198	1	100	3.1	7141	PASS
441	198	0.01	100	12.3	28347	PASS
442	442	50	100	100.0	182312	PASS
443	442	15	24	19.6	35687	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012722\
 Data File : BF126704.D
 Acq On : 27 Jan 2022 09:50
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Jan 28 06:12:21 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jan 27 03:09:40 2022
 Response via : Initial Calibration

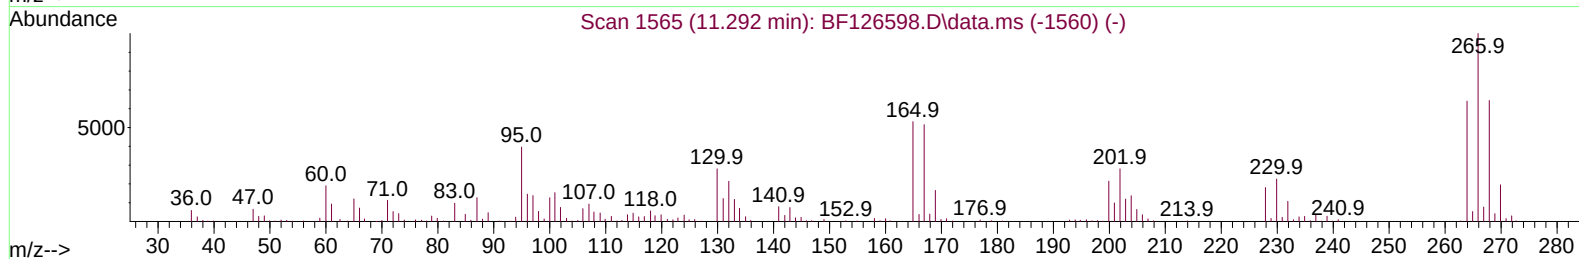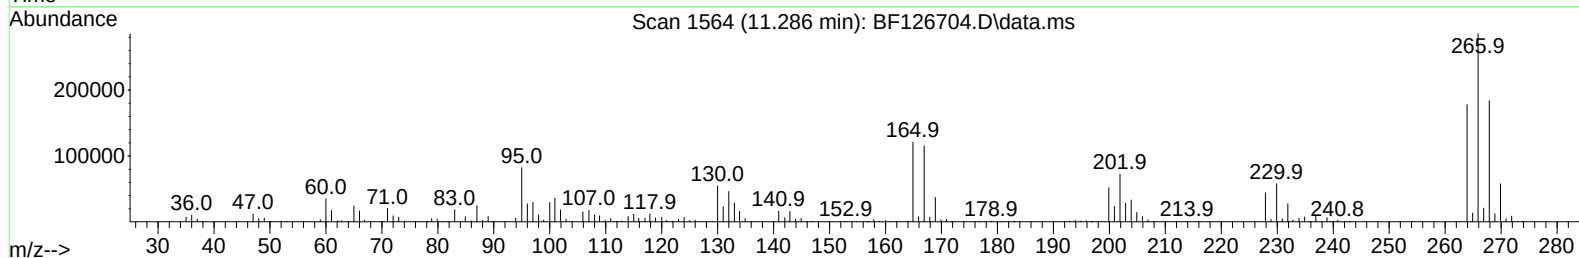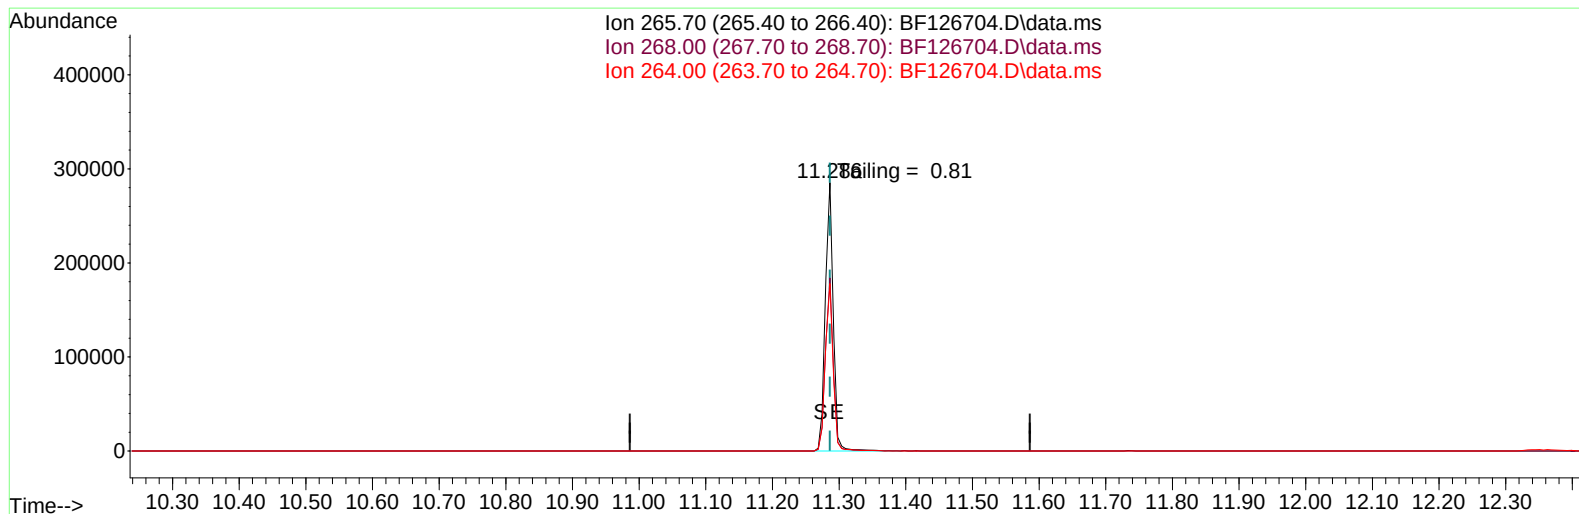

TIC: BF126704.D\data.ms

(70) Pentachlorophenol (C)

11.286min (-0.000) 32095.38 ng

response 235459

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.40	64.45
264.00	63.00	62.35
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
1/27/2022	BNA_F	<u>BF126704.D</u>
Compound Name	Response	Retention Time
DDT	598663	13.657
DDD	7664	13.351
DDE	907	13.015
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
8571	607234	1.41

Instrument :
BNA_F
ClientSampleId :
DFTPP