
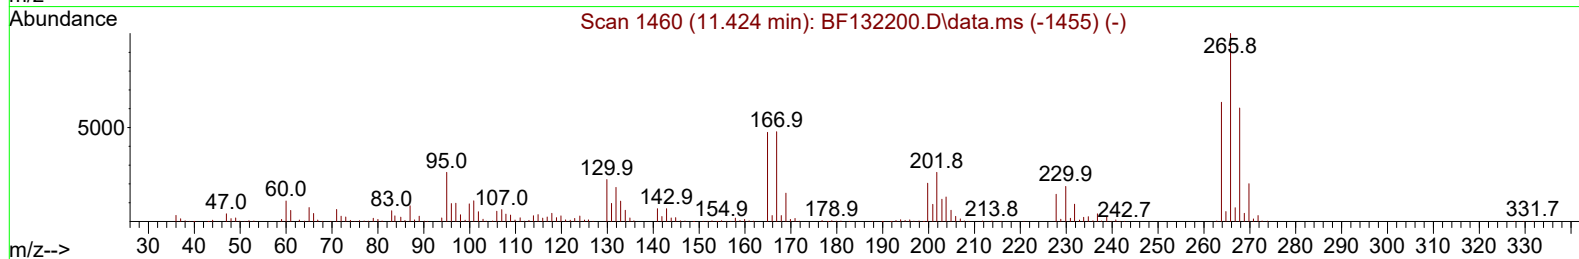
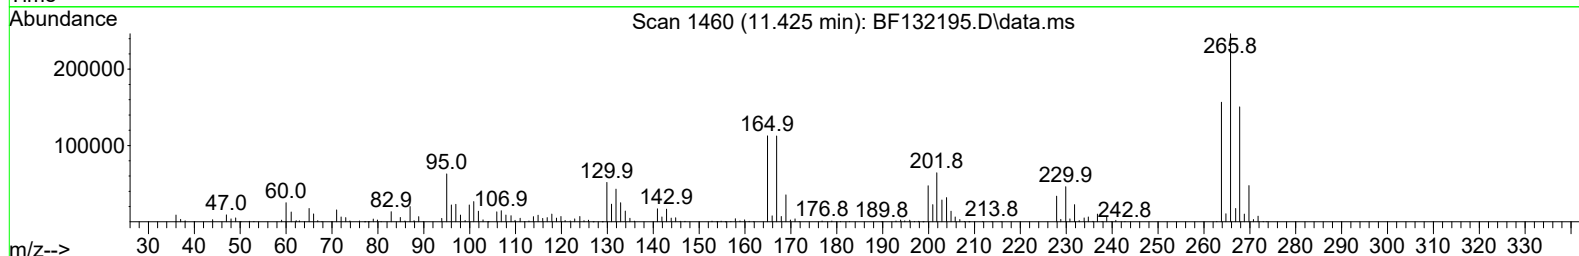


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012723\
Data File : BF132195.D
Acq On : 27 Jan 2023 12:03
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 28 04:45:20 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF012723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jan 28 02:25:45 2023
Response via : Initial Calibration

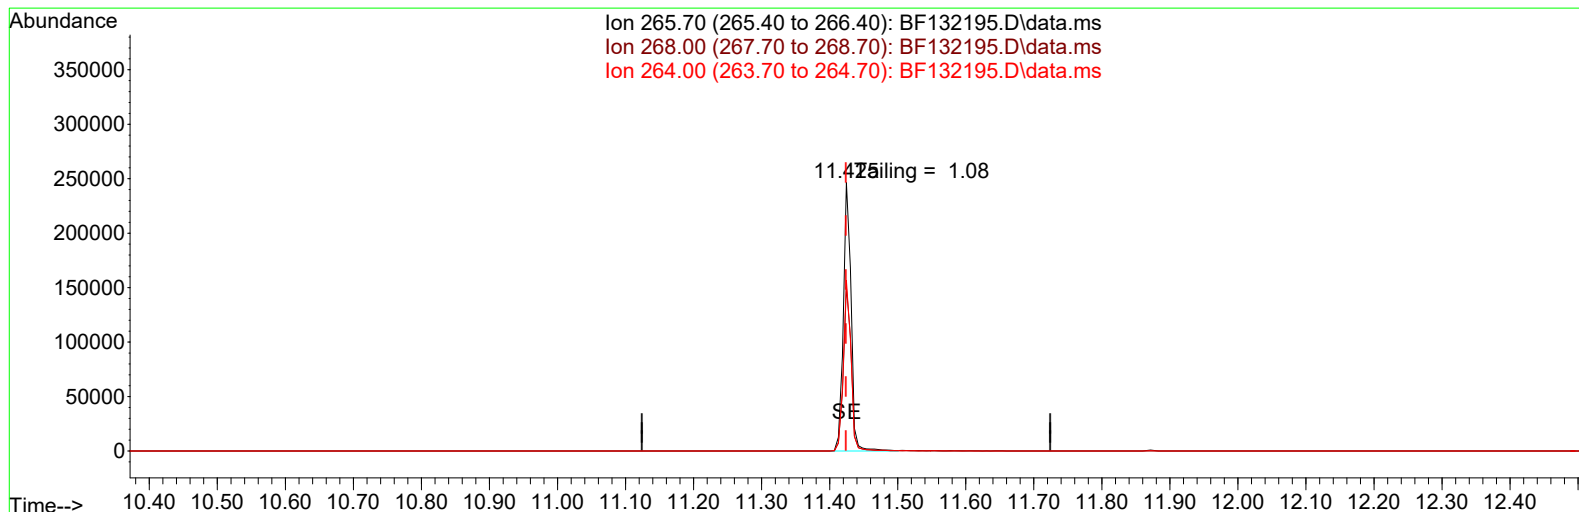

TIC: BF132195.D\data.ms

(70) Pentachlorophenol (C)




11.425min (+ 0.001) 22702.09 ng

response 195369

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	60.30	61.14
264.00	63.40	63.58
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012723\
Data File : BF132195.D
Acq On : 27 Jan 2023 12:03
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 28 04:45:20 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF012723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jan 28 02:25:45 2023
Response via : Initial Calibration

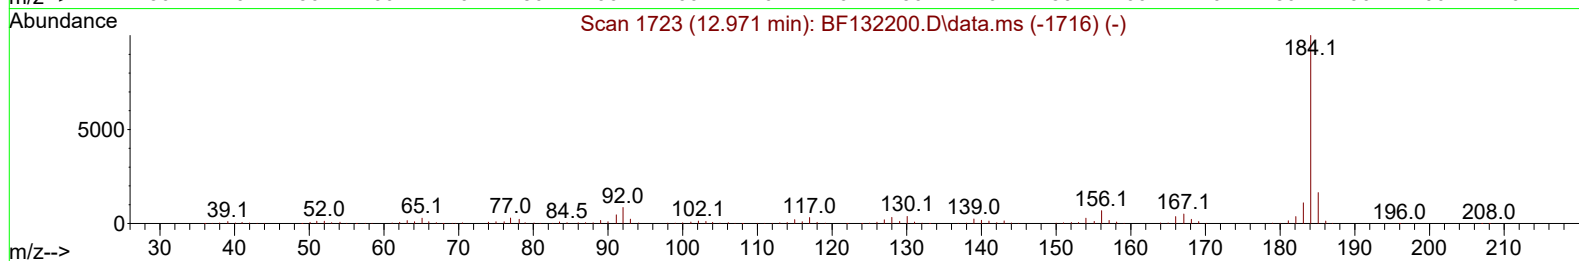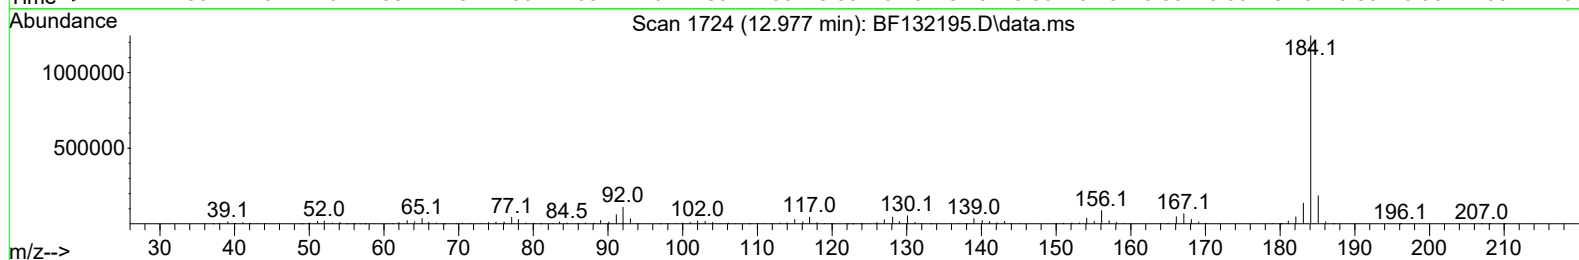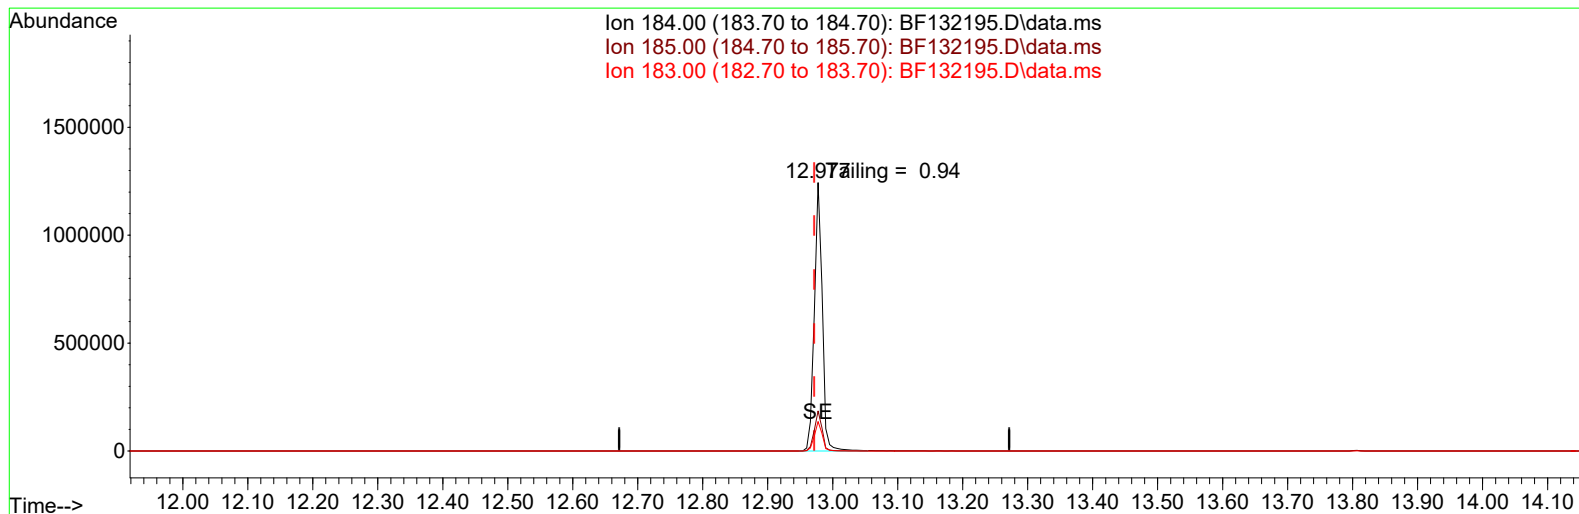

TIC: BF132195.D\data.ms

(77) Benzidine

12.977min (+ 0.006) 0.00 ng

response 1061100

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	16.50	14.90
183.00	11.00	10.98
0.00	0.00	0.00