
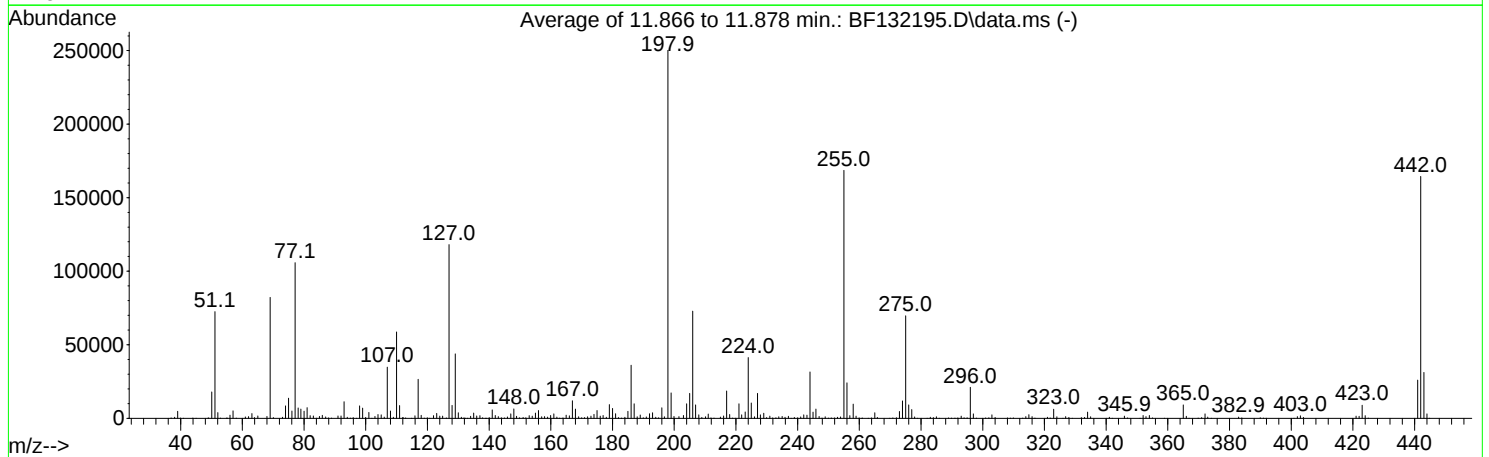


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012723\
Data File : BF132195.D
Acq On : 27 Jan 2023 12:03
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF012723.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Sat Jan 28 02:25:45 2023

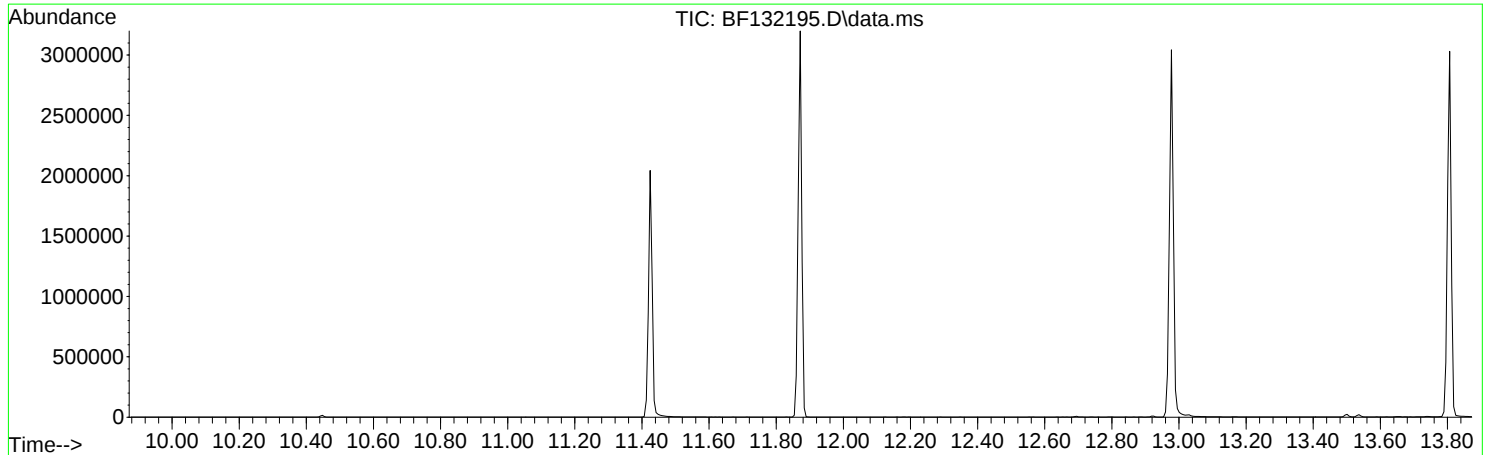




AutoFind: Scans 1535, 1536, 1537; Background Corrected with Scan 1530

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.0	72485	PASS
68	69	0.00	2	1.5	1256	PASS
69	198	0.00	100	32.9	82184	PASS
70	69	0.00	2	0.5	452	PASS
127	198	10	80	47.2	118064	PASS
197	198	0.00	2	0.4	993	PASS
198	198	100	100	100.0	250112	PASS
199	198	5	9	6.9	17253	PASS
275	198	10	60	27.9	69680	PASS
365	198	1	100	3.6	9085	PASS
441	198	0.01	100	10.4	26012	PASS
442	442	50	100	100.0	164475	PASS
443	442	15	24	19.0	31218	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012723\
 Data File : BF132195.D
 Acq On : 27 Jan 2023 12:03
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Jan 28 04:45:20 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF012723.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Jan 28 02:25:45 2023
 Response via : Initial Calibration

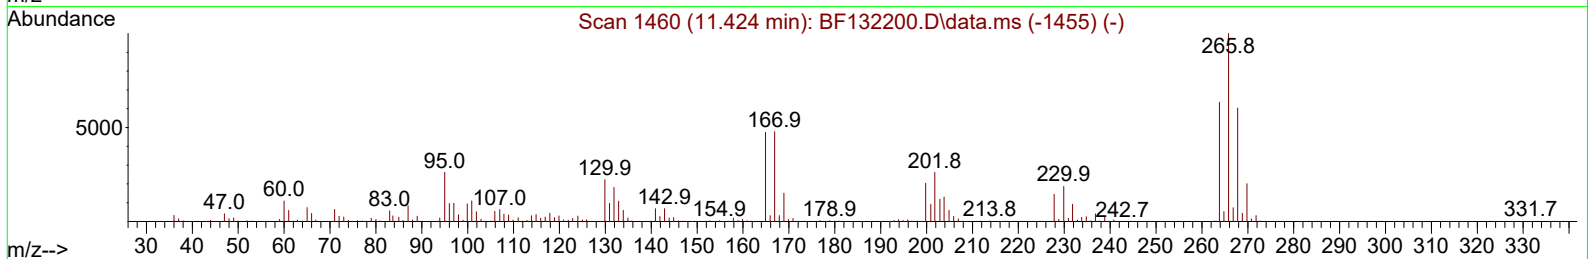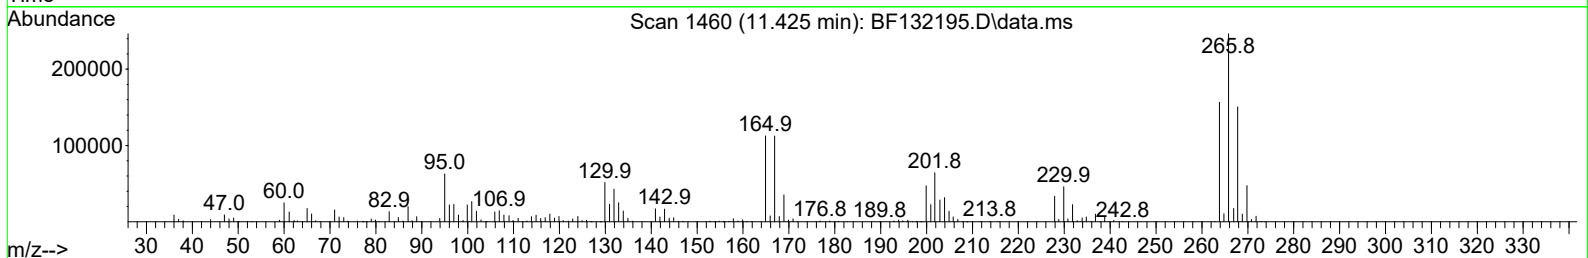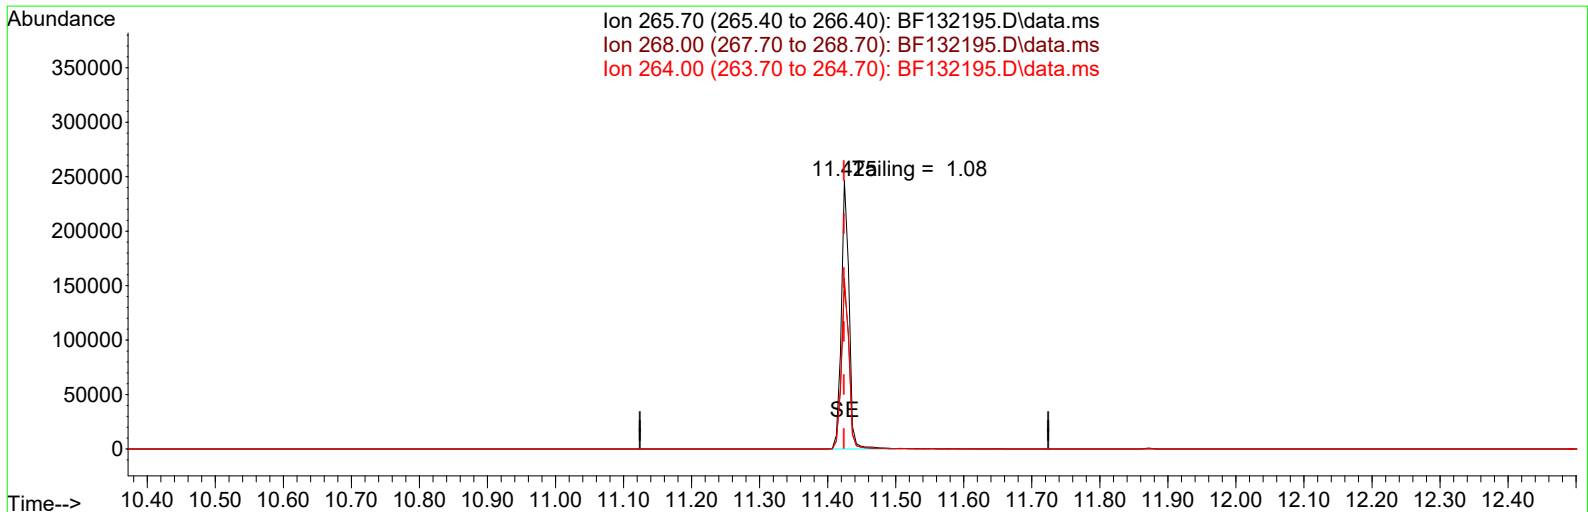

TIC: BF132195.D\data.ms

(70) Pentachlorophenol (C)

11.425min (+ 0.001) 22702.09 ng




response 195369

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	60.30	61.14
264.00	63.40	63.58
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012723\
Data File : BF132195.D
Acq On : 27 Jan 2023 12:03
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jan 28 04:45:20 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF012723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jan 28 02:25:45 2023
Response via : Initial Calibration

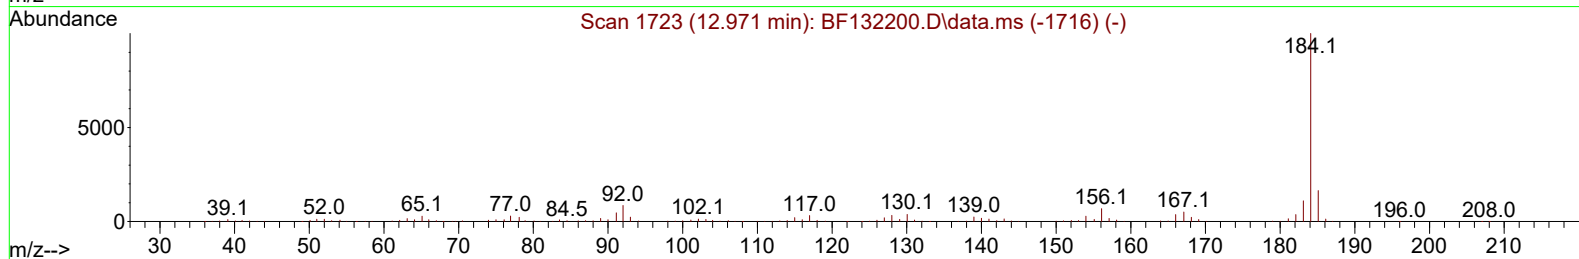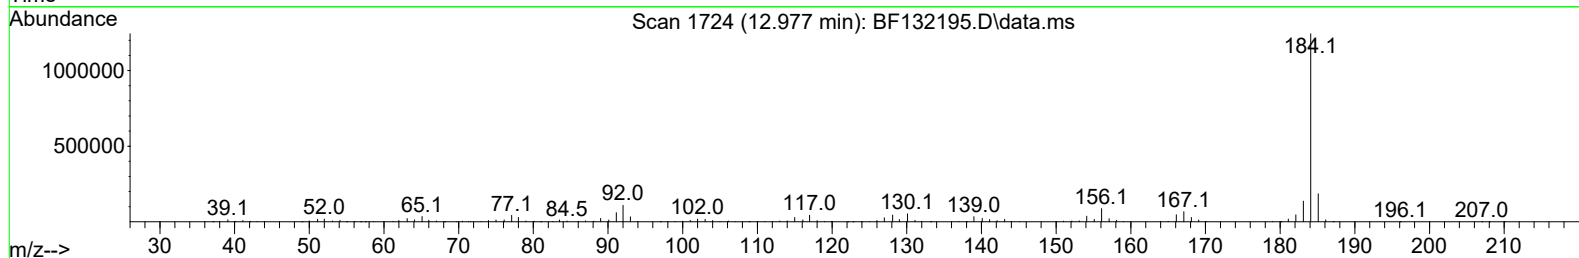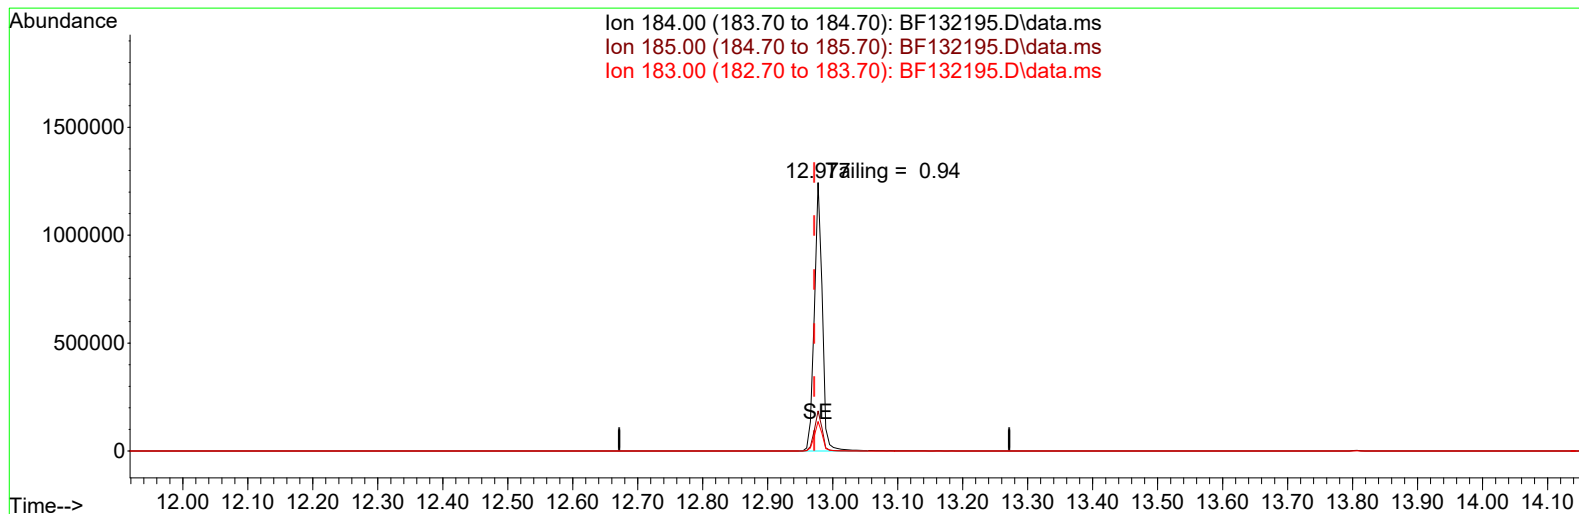

TIC: BF132195.D\data.ms

(77) Benzidine

12.977min (+ 0.006) 0.00 ng

response 1061100

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	16.50	14.90
183.00	11.00	10.98
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
1/27/2023	BNA_F	<u>BF132195.D</u>
Compound Name	Response	Retention Time
DDT	399685	13.807
DDD	6435	13.501
DDE	296	13.16
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6731	406416	1.66

Instrument :
BNA_F
ClientSampleId :
DFTPP