

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012725\
 Data File : BF141276.D
 Acq On : 27 Jan 2025 16:51
 Operator : RC/JU
 Sample : Q1169-04
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 REGULATOR-BUILDING-GRAVEL

Quant Time: Jan 27 17:38:51 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011025.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jan 10 22:54:19 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.804	152	136506	20.000	ng	-0.02
21) Naphthalene-d8	8.081	136	541009	20.000	ng	-0.02
39) Acenaphthene-d10	9.839	164	273744	20.000	ng	-0.02
64) Phenanthrene-d10	11.328	188	440856	20.000	ng	-0.02
76) Chrysene-d12	13.969	240	330892	20.000	ng	-0.02
86) Perylene-d12	15.439	264	286824	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.428	112	1046245	118.401	ng	0.00
7) Phenol-d6	6.434	99	1258650	112.447	ng	-0.01
23) Nitrobenzene-d5	7.363	82	838384	82.145	ng	-0.02
42) 2,4,6-Tribromophenol	10.633	330	456778	146.444	ng	-0.02
45) 2-Fluorobiphenyl	9.163	172	1601542	89.340	ng	-0.02
79) Terphenyl-d14	12.922	244	1850683	83.129	ng	-0.01


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012725\
Data File : BF141276.D
Acq On : 27 Jan 2025 16:51
Operator : RC/JU
Sample : Q1169-04
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
REGULATOR-BUILDING-GRAVEL

Quant Time: Jan 27 17:38:51 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 10 22:54:19 2025
Response via : Initial Calibration




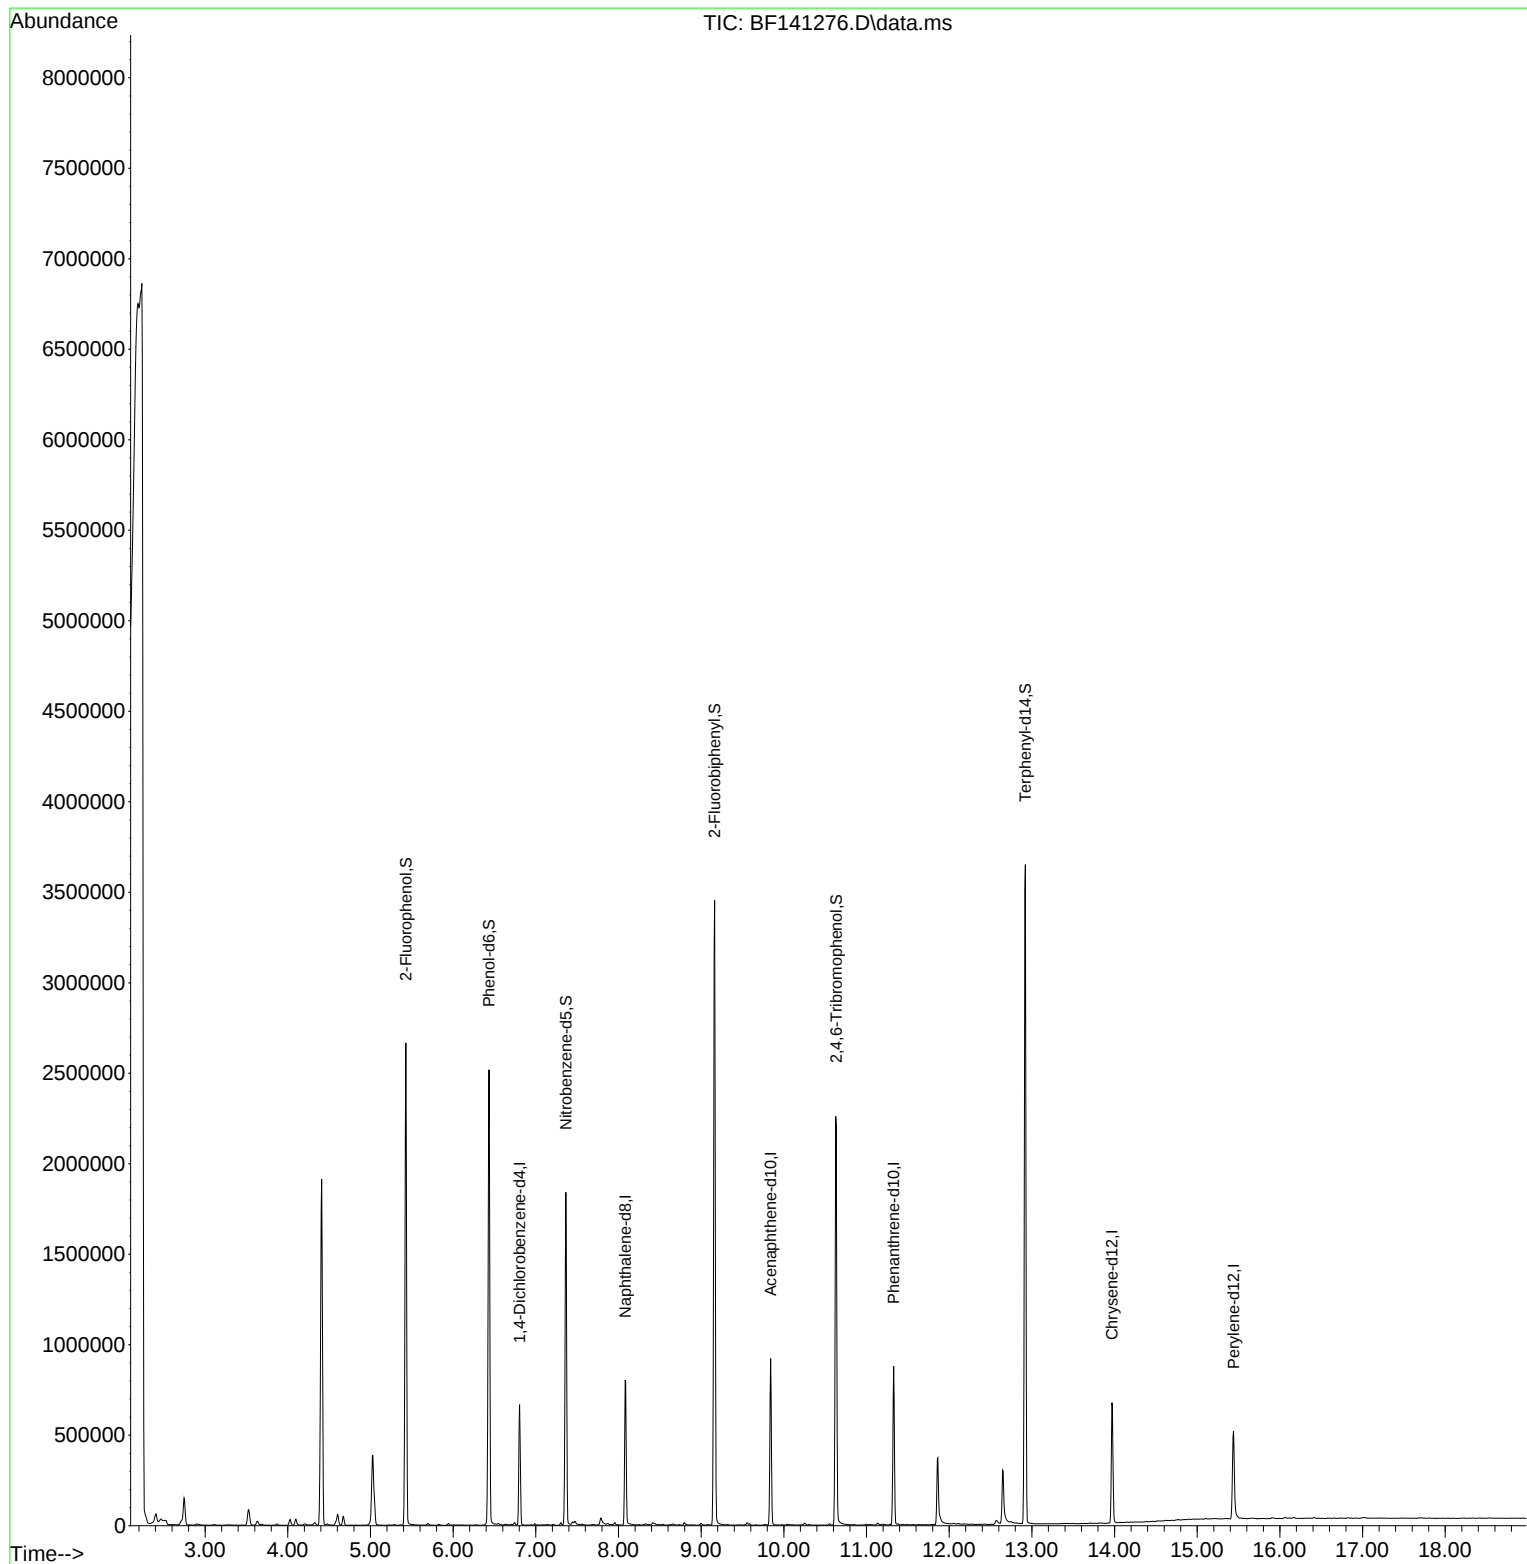


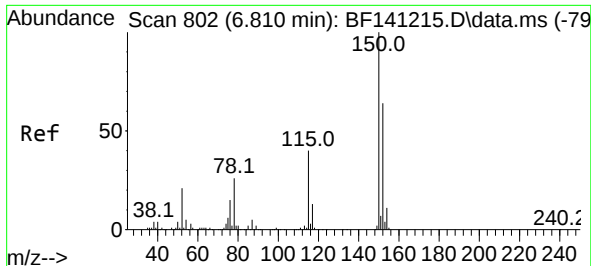

#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.804 min Scan# 801
Delta R.T. -0.018 min
Lab File: BF141276.D
Acq: 27 Jan 2025 16:51




Instrument :
BNA_F
ClientSampleId :
REGULATOR-BUILDING-GRAVEL


Tgt Ion:152 Resp: 136506
Ion Ratio Lower Upper
152 100
150 155.7 125.8 188.8
115 63.0 51.4 77.2

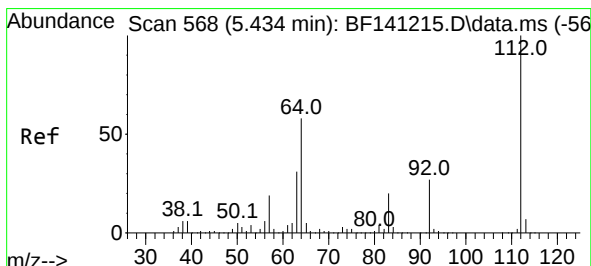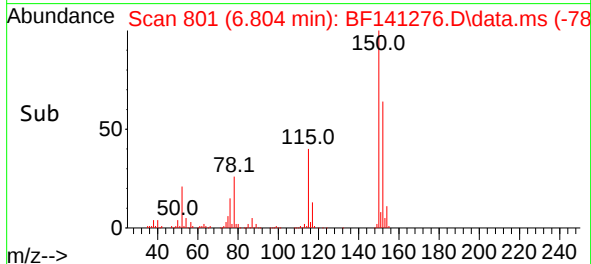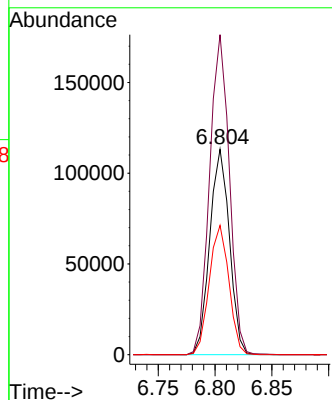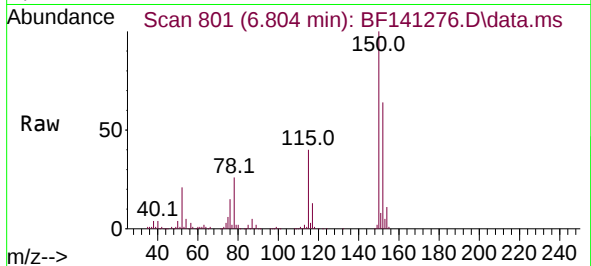

#5
2-Fluorophenol
Concen: 118.401 ng
RT: 5.428 min Scan# 567
Delta R.T. 0.000 min
Lab File: BF141276.D
Acq: 27 Jan 2025 16:51


Tgt Ion:112 Resp: 1046245
Ion Ratio Lower Upper
112 100
64 56.8 47.3 70.9
63 29.7 24.2 36.2

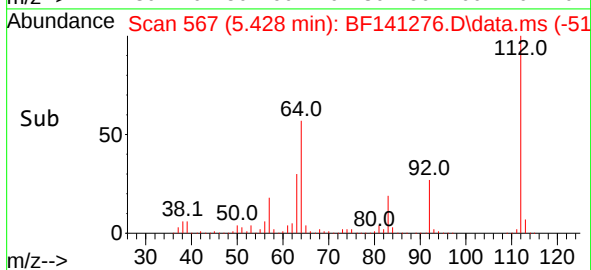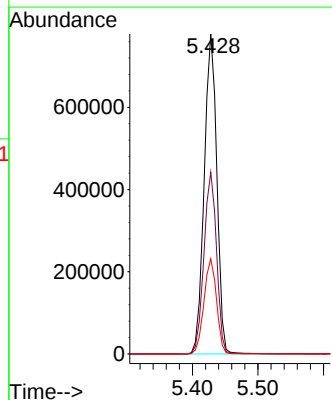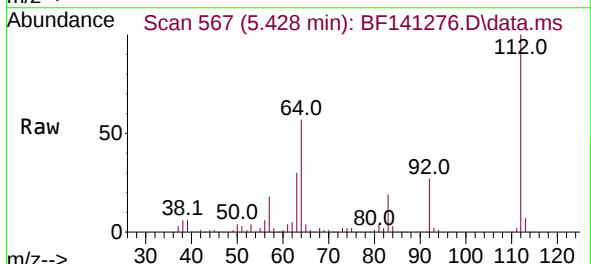



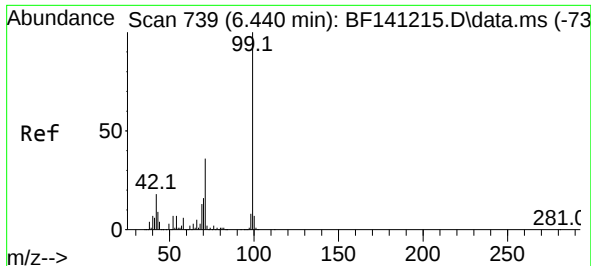


#7
Phenol-d6
Concen: 112.447 ng
RT: 6.434 min Scan# 71
Delta R.T. -0.012 min
Lab File: BF141276.D
Acq: 27 Jan 2025 16:51

Instrument :
BNA_F
ClientSampleId :
REGULATOR-BUILDING-GRAVEL



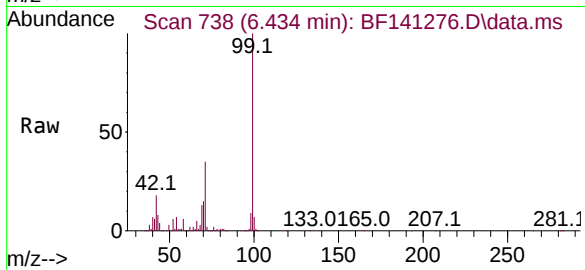



Tgt Ion: 99 Resp: 1258650
Ion Ratio Lower Upper
99 100
42 17.5 15.0 22.4
71 34.7 27.6 41.4

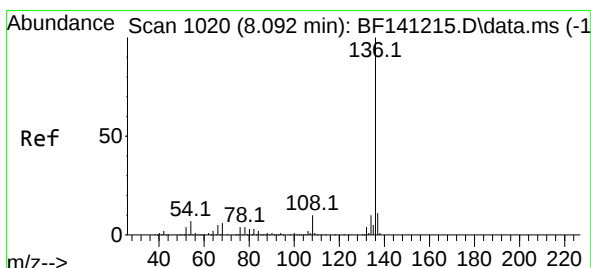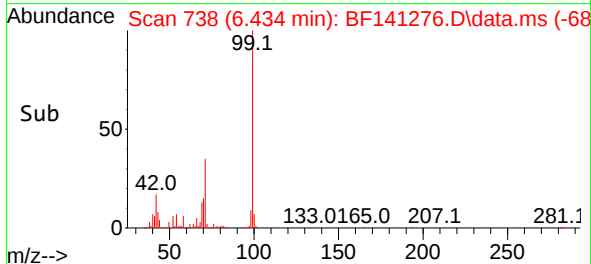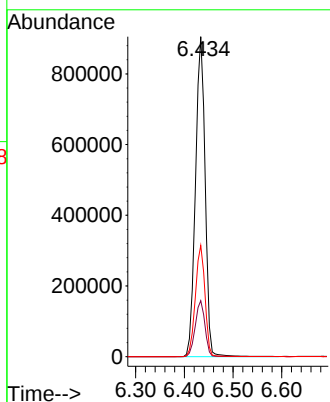

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.081 min Scan# 1018
Delta R.T. -0.023 min
Lab File: BF141276.D
Acq: 27 Jan 2025 16:51

Tgt Ion:136 Resp: 541009
Ion Ratio Lower Upper
136 100
137 11.1 8.8 13.2
54 7.8 6.3 9.5
68 5.8 4.9 7.3


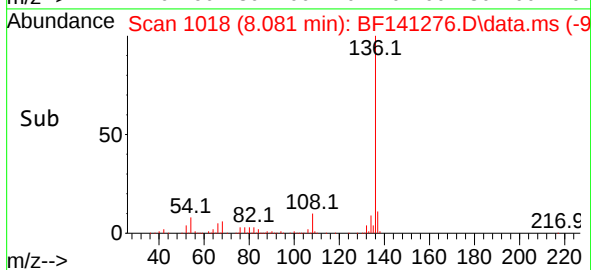
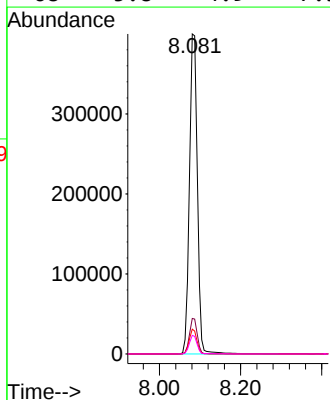
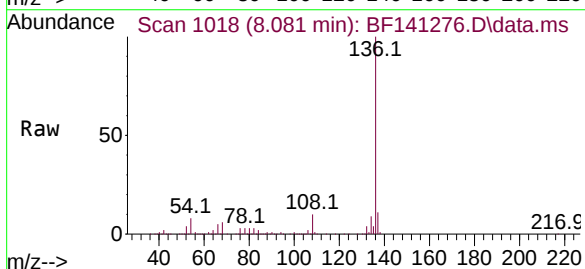


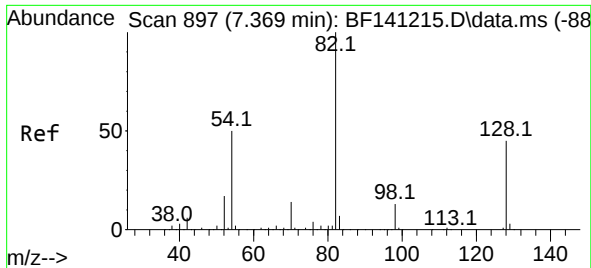

#23
Nitrobenzene-d5
Concen: 82.145 ng
RT: 7.363 min Scan# 897
Delta R.T. -0.023 min
Lab File: BF141276.D
Acq: 27 Jan 2025 16:51




Instrument :
BNA_F
ClientSampleId :
REGULATOR-BUILDING-GRAVEL


Tgt Ion: 82 Resp: 838384
Ion Ratio Lower Upper
82 100
128 46.4 36.1 54.1
54 49.3 41.0 61.4

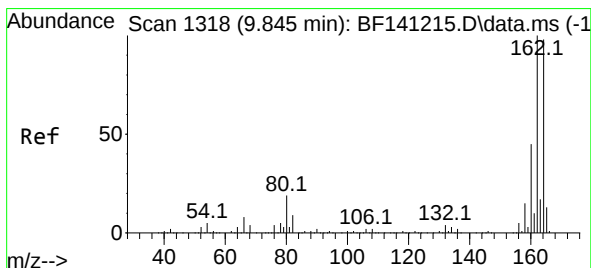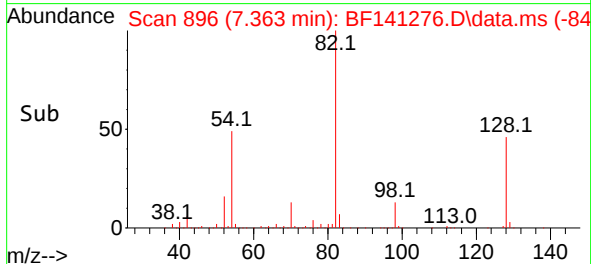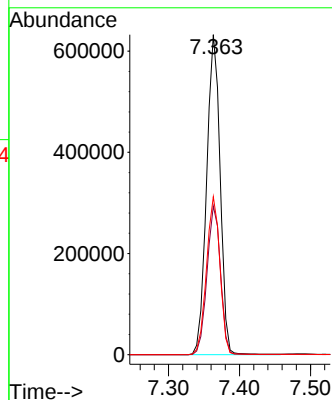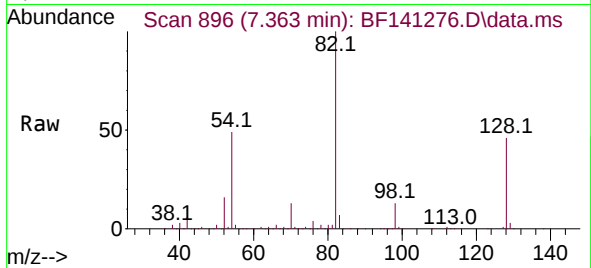

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.839 min Scan# 1317
Delta R.T. -0.023 min
Lab File: BF141276.D
Acq: 27 Jan 2025 16:51

Tgt Ion:164 Resp: 273744
Ion Ratio Lower Upper
164 100
162 100.8 81.0 121.4
160 44.7 36.1 54.1


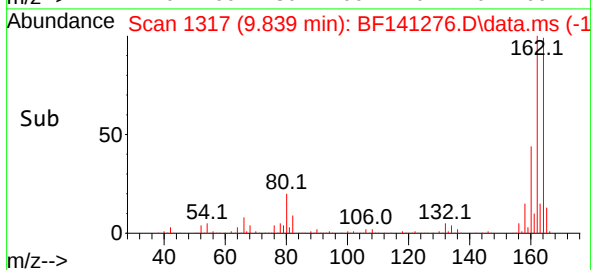
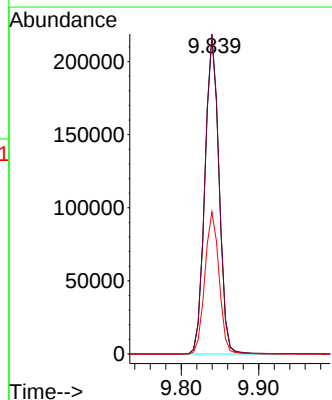
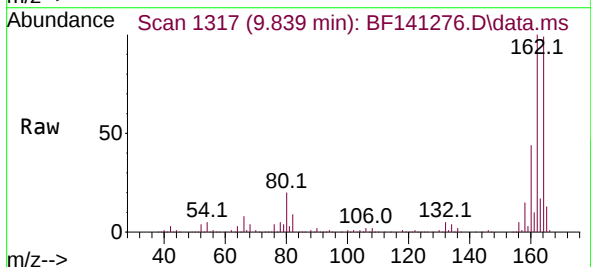


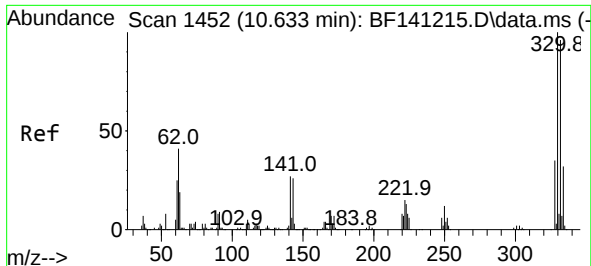

#42
 2,4,6-Tribromophenol
 Concen: 146.444 ng
 RT: 10.633 min Scan# 1452
 Delta R.T. -0.018 min
 Lab File: BF141276.D
 Acq: 27 Jan 2025 16:51




Instrument :
 BNA_F
 ClientSampleId :
 REGULATOR-BUILDING-GRAVEL


Tgt Ion: 330 Resp: 456778
 Ion Ratio Lower Upper
 330 100
 332 96.7 76.9 115.3
 141 27.7 25.2 37.8

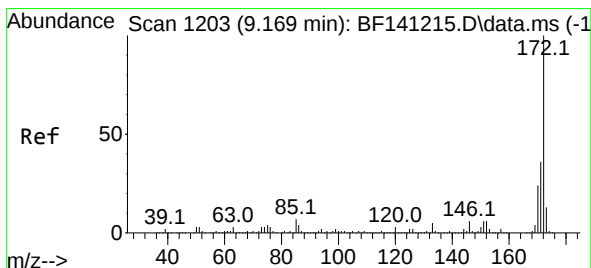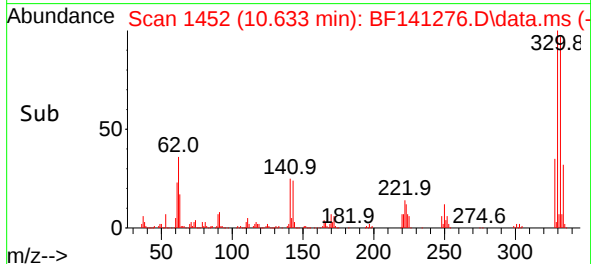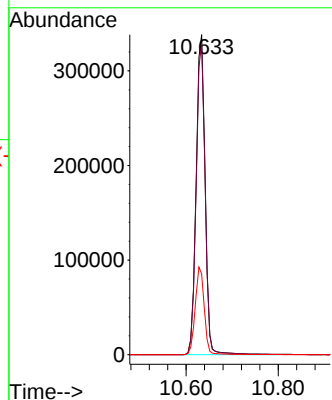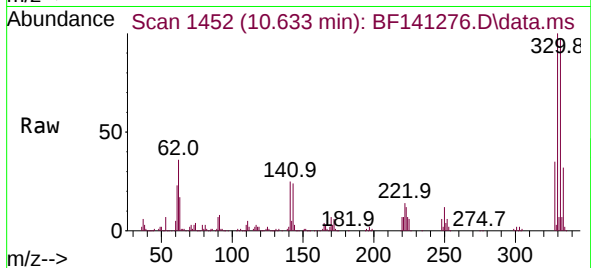

#45
 2-Fluorobiphenyl
 Concen: 89.340 ng
 RT: 9.163 min Scan# 1202
 Delta R.T. -0.018 min
 Lab File: BF141276.D
 Acq: 27 Jan 2025 16:51

Tgt Ion: 172 Resp: 1601542
 Ion Ratio Lower Upper
 172 100
 171 35.7 28.7 43.1
 170 23.3 19.0 28.6

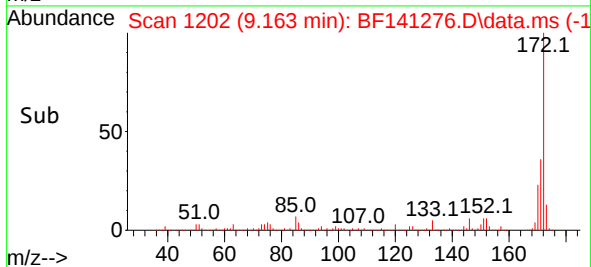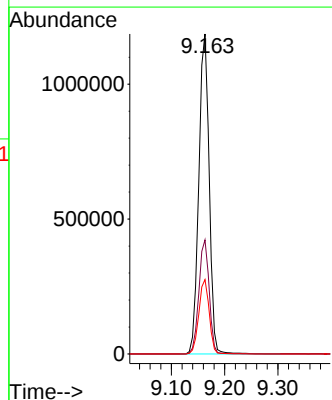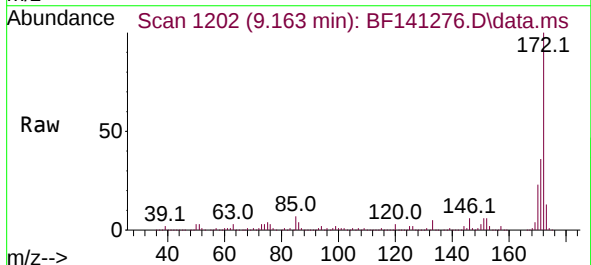

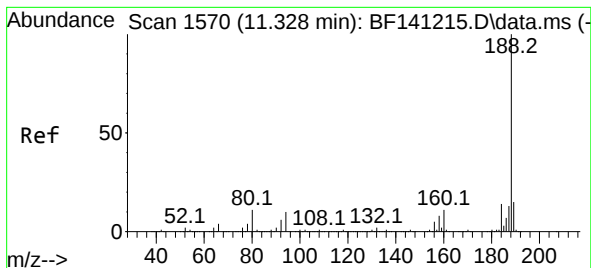

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 11.328 min Scan# 1

Delta R.T. -0.018 min

Lab File: BF141276.D

Acq: 27 Jan 2025 16:51

Instrument :

BNA_F

ClientSampleId :

REGULATOR-BUILDING-GRAVEL





Tgt Ion:188 Resp: 440856

Ion Ratio Lower Upper

188 100

94 9.6 8.3 12.5

80 10.4 9.0 13.4

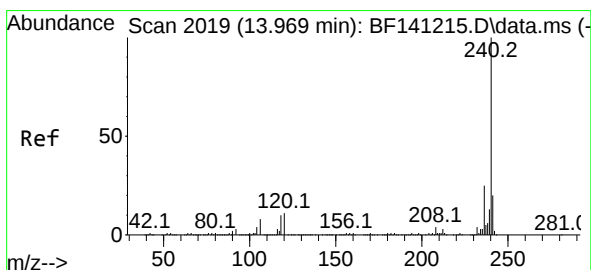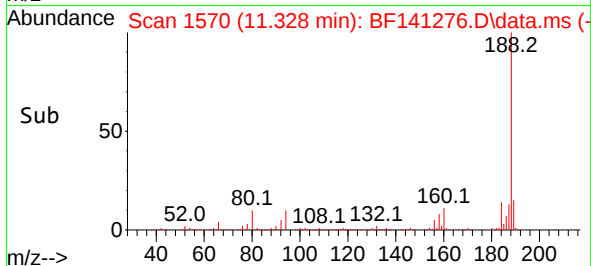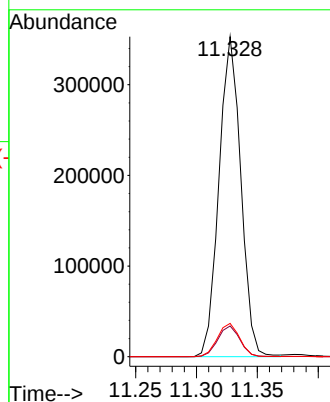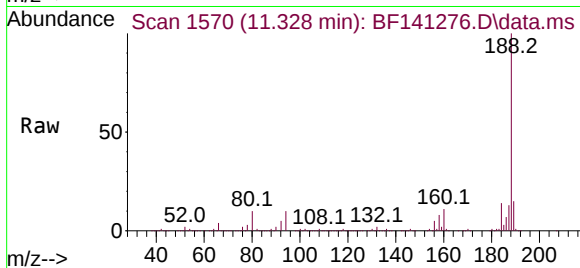

#76

Chrysene-d12

Concen: 20.000 ng

RT: 13.969 min Scan# 2019

Delta R.T. -0.018 min

Lab File: BF141276.D

Acq: 27 Jan 2025 16:51




Tgt Ion:240 Resp: 330892


Ion Ratio Lower Upper

240 100

120 11.5 9.1 13.7


236 25.2 19.8 29.6

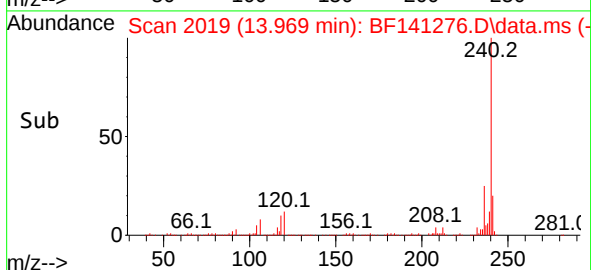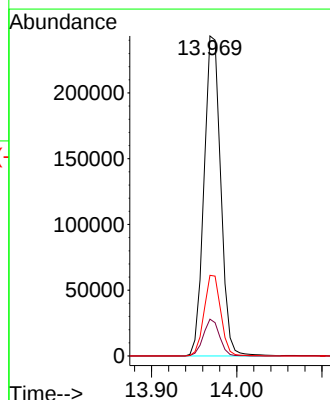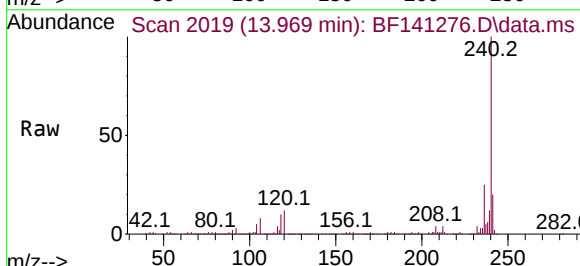



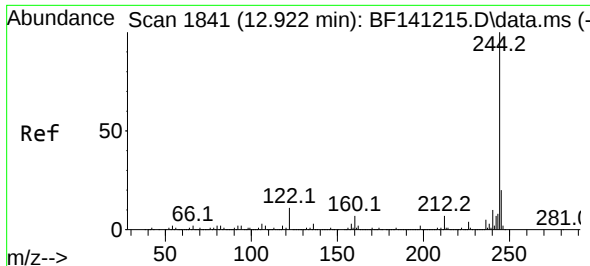


#79
 Terphenyl-d14
 Concen: 83.129 ng
 RT: 12.922 min Scan# 1841
 Delta R.T. -0.012 min
 Lab File: BF141276.D
 Acq: 27 Jan 2025 16:51


Instrument : BNA_F
 ClientSampleId : REGULATOR-BUILDING-GRAVEL

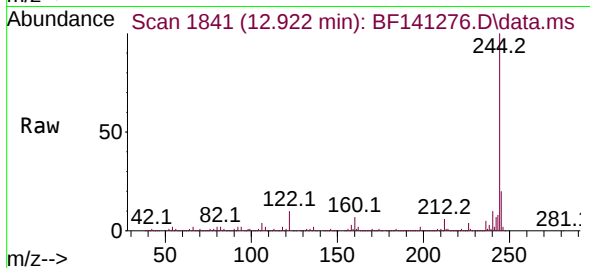

Tgt Ion:244 Resp: 1850683
 Ion Ratio Lower Upper
 244 100
 212 6.5 5.4 8.2
 122 10.4 8.8 13.2

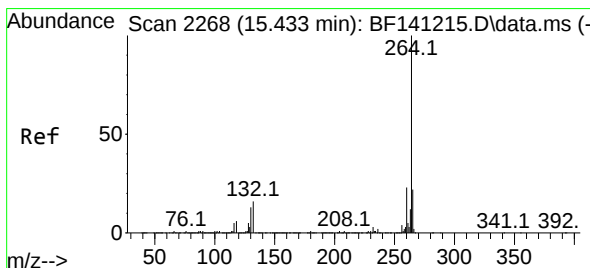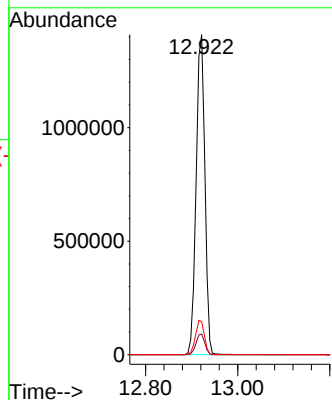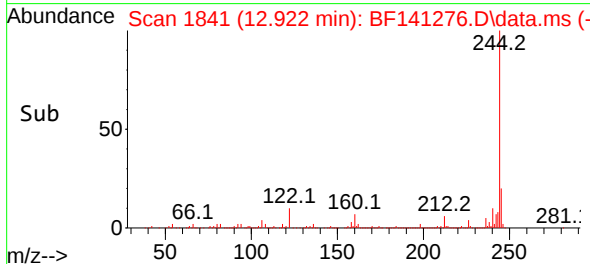

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.439 min Scan# 2269
 Delta R.T. 0.000 min
 Lab File: BF141276.D
 Acq: 27 Jan 2025 16:51

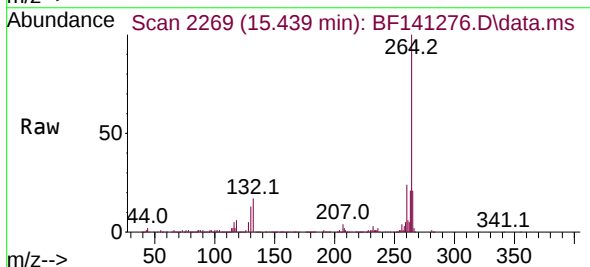

Tgt Ion:264 Resp: 286824
 Ion Ratio Lower Upper
 264 100
 260 23.9 18.6 28.0
 265 21.4 17.4 26.0

