


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012725\
Data File : BF141265.D
Acq On : 27 Jan 2025 11:32
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011025.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Jan 10 22:54:19 2025

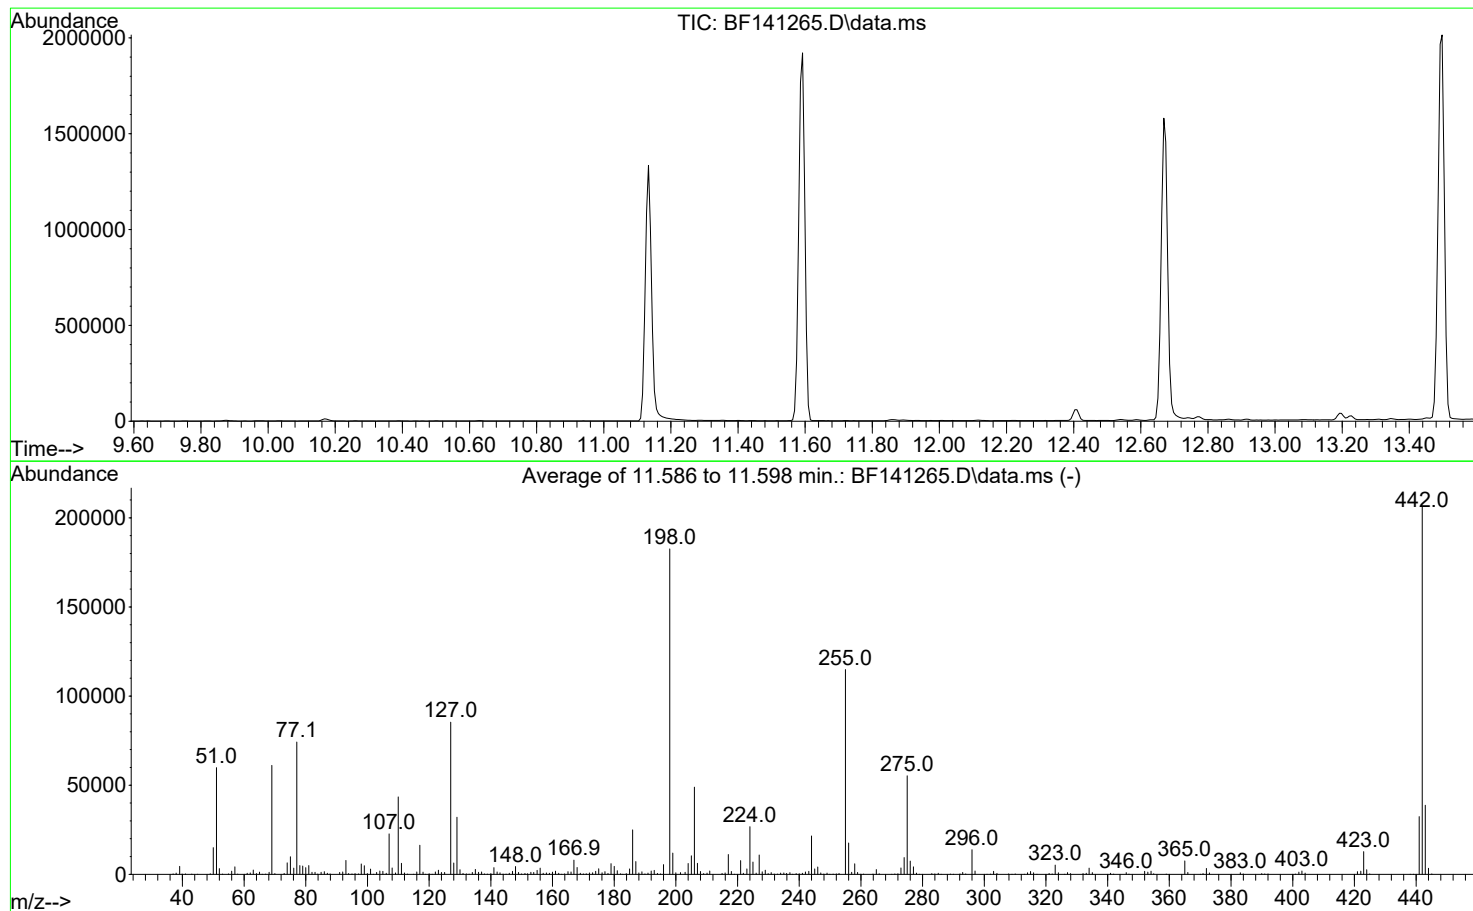

AutoFind: Scans 1614, 1615, 1616; Background Corrected with Scan 1607

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.8	59872	PASS
68	69	0.00	2	1.9	1148	PASS
69	198	0.00	100	33.5	61125	PASS
70	69	0.00	2	0.7	445	PASS
127	198	10	80	46.8	85360	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	182528	PASS
199	198	5	9	6.6	11977	PASS
275	198	10	60	30.3	55331	PASS
365	198	1	100	4.1	7556	PASS
441	198	0.01	100	17.7	32376	PASS
442	442	50	100	100.0	206357	PASS
443	442	15	24	18.8	38781	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
1/27/2025	BNA_F	<u>BF141265.D</u>
Compound Name	Response	Retention Time
DDT	534048	13.498
DDD	15464	13.192
DDE	1419	12.857
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
16883	550931	3.06

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012725\
Data File : BF141265.D
Acq On : 27 Jan 2025 11:32
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jan 27 12:26:52 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 10 22:54:19 2025
Response via : Initial Calibration

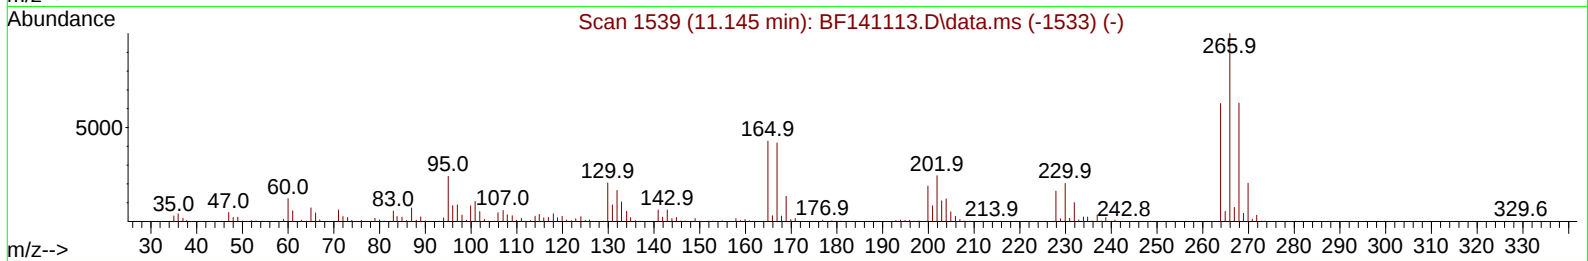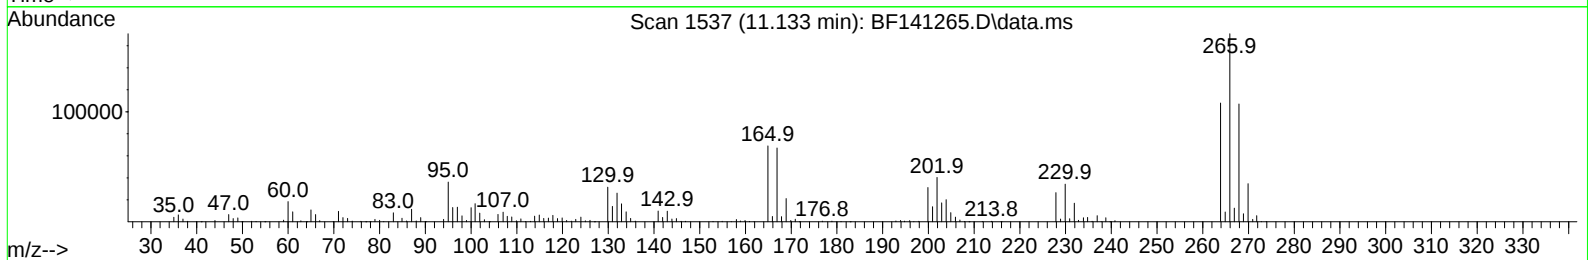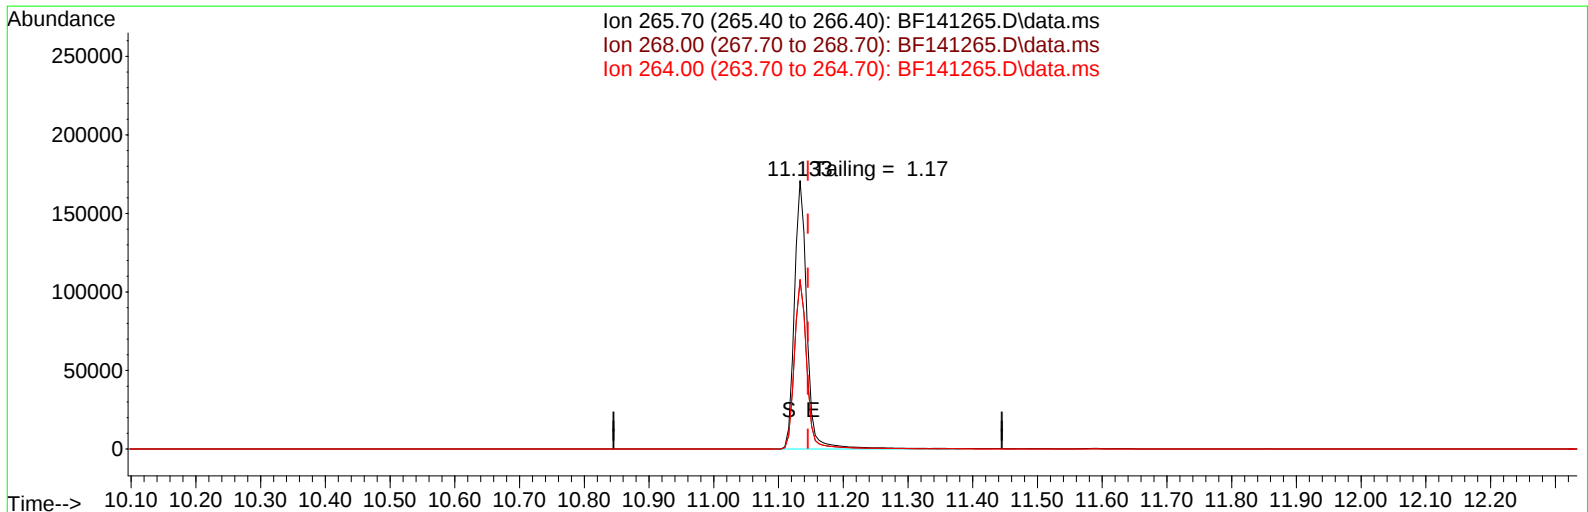

TIC: BF141265.D\data.ms

(70) Pentachlorophenol (C)

11.133min (-0.012) 23981.38 ng




response 229106

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.00	62.71
264.00	62.70	63.18
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012725\
Data File : BF141265.D
Acq On : 27 Jan 2025 11:32
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jan 27 12:26:52 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 10 22:54:19 2025
Response via : Initial Calibration

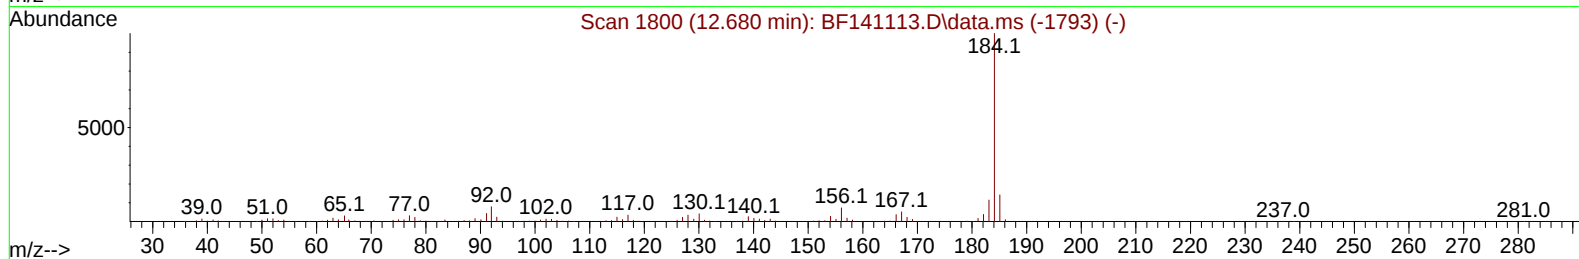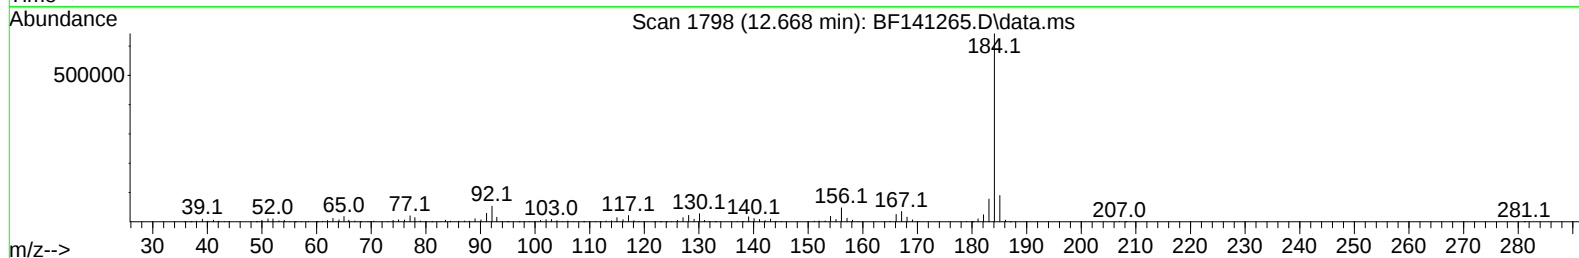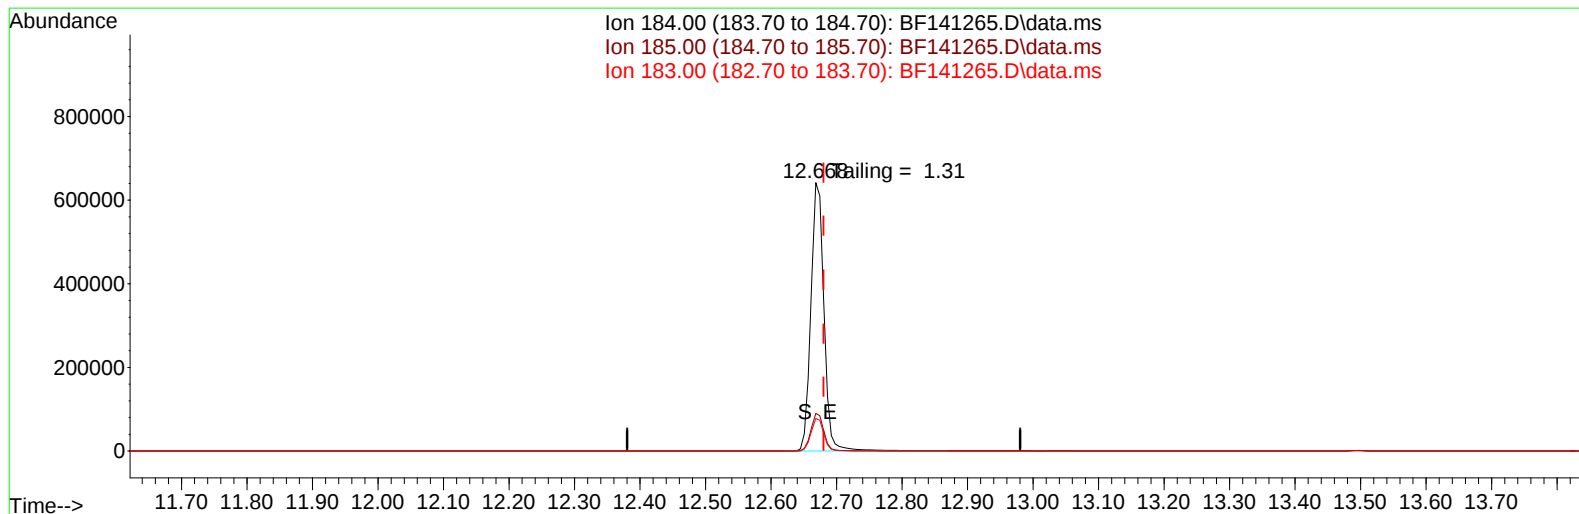

TIC: BF141265.D\data.ms

(77) Benzidine

12.668min (-0.012) 58178.64 ng

response 885766

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	14.01
183.00	11.50	12.12
0.00	0.00	0.00