

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF012815\
 Data File : BF077101.D
 Acq On : 28 Jan 2015 14:37
 Operator : TP/IZ
 Sample : G1175-05
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SVOC-GPC-BLANK

Quant Time: Jan 29 00:03:40 2015
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF011415.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jan 28 16:07:35 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.72	152	21347	20.00	ng	0.00
21) Naphthalene-d8	10.63	136	88521	20.00	ng	0.00
38) Acenaphthene-d10	14.75	164	48258	20.00	ng	-0.01
63) Phenanthrene-d10	17.59	188	80928	20.00	ng	-0.01
75) Chrysene-d12	21.10	240	80147	20.00	ng	-0.01
86) Perylene-d12	22.75	264	73579	20.00	ng	-0.07

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units
5) 2-Fluorophenol	0.00	112	0	0.00	ng
7) Phenol-d6	0.00	99	0	0.00	ng
23) Nitrobenzene-d5	0.00	82	0	0.00	ng
41) 2,4,6-Tribromophenol	0.00	330	0	0.00	ng
44) 2-Fluorobiphenyl	0.00	172	0	0.00	ng
78) Terphenyl-d14	0.00	244	0	0.00	ng


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF012815\
Data File : BF077101.D
Acq On : 28 Jan 2015 14:37
Operator : TP/IZ
Sample : G1175-05
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SVOC-GPC-BLANK

Quant Time: Jan 29 00:03:40 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF011415.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 28 16:07:35 2015
Response via : Initial Calibration

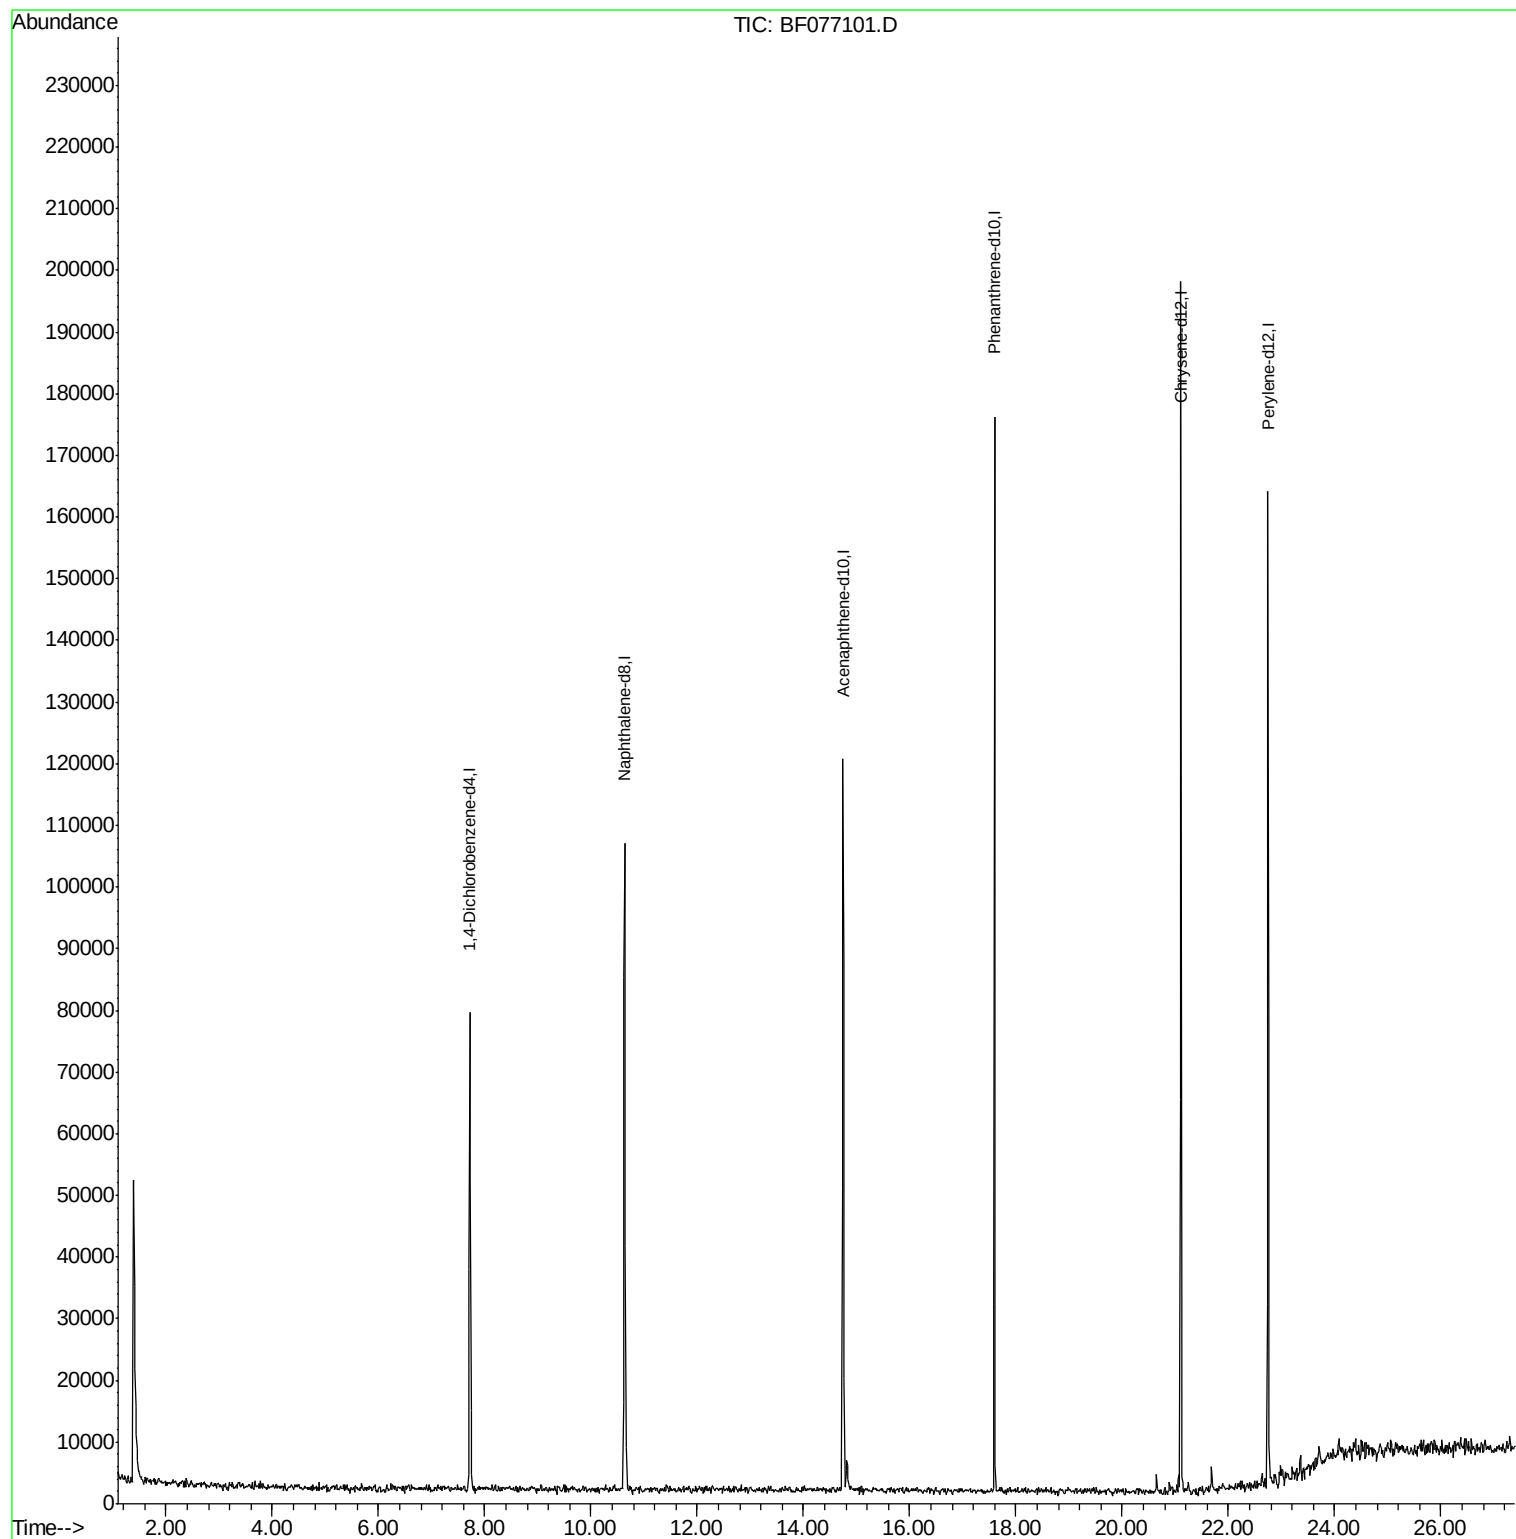

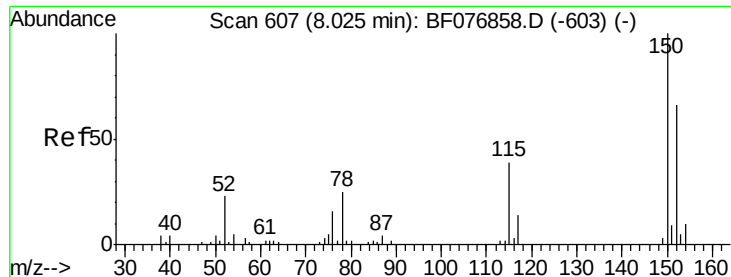


#1




1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 7.72 min Scan# 580
Delta R.T. -0.00 min
Lab File: BF077101.D
Acq: 28 Jan 2015 14:37

Instrument :
BNA_F
ClientSampleId :
SVOC-GPC-BLANK

Tgt Ion:152 Resp: 21347
Ion Ratio Lower Upper
152 100
150 164.0 121.7 182.5
115 60.5 47.0 70.6

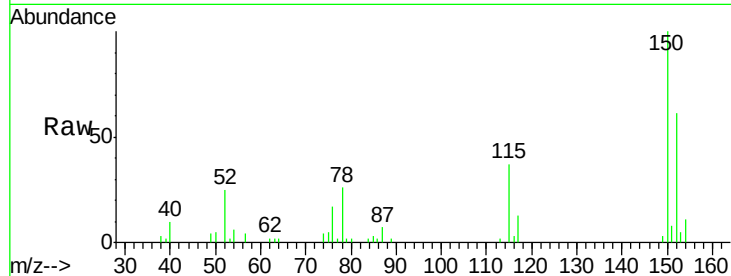

Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

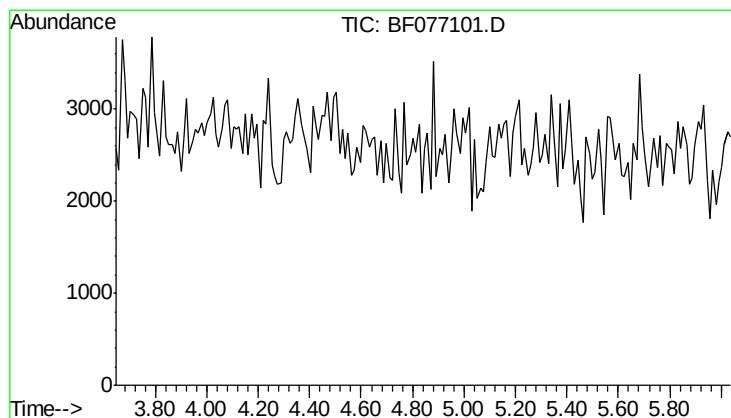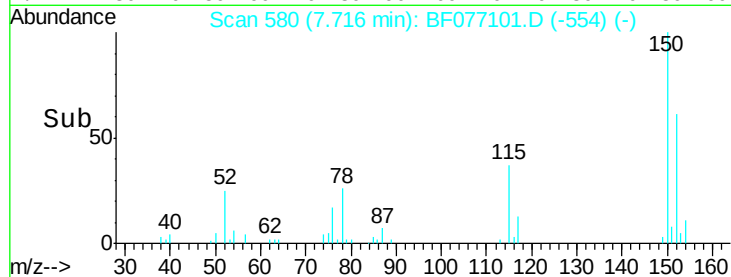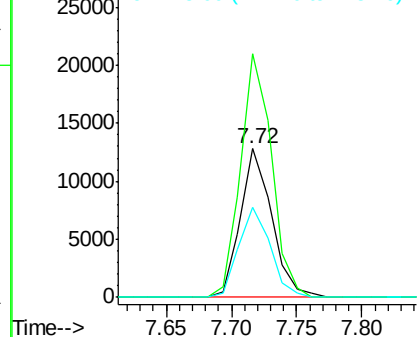



#5

2-Fluorophenol
Concen: 0.00 ng
Expected RT: 4.74 min

Lab File: BF077101.D
Acq: 28 Jan 2015 14:37

Tgt Ion: 112
Sig Exp Ratio
112 100
64 67.8
63 35.5

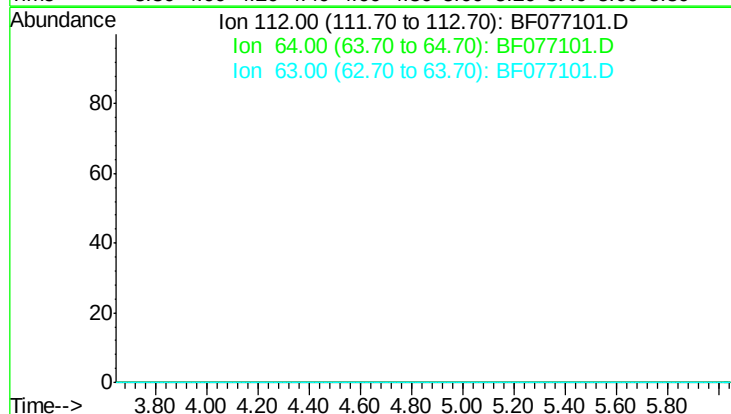

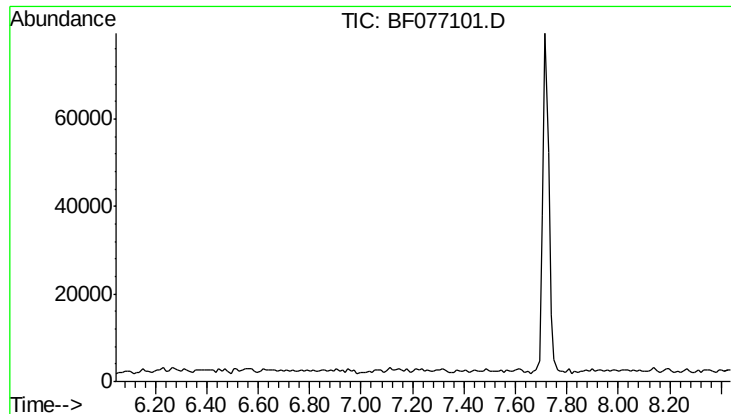

#7

Phenol-d6

Concen: 0.00 ng

Expected RT: 7.14 min

Lab File: BF077101.D

Acq: 28 Jan 2015 14:37

Instrument :

BNA_F

ClientSampleId :

SVOC-GPC-BLANK



Tgt Ion: 99

Sig Exp Ratio

99 100

42 18.7

71 38.1

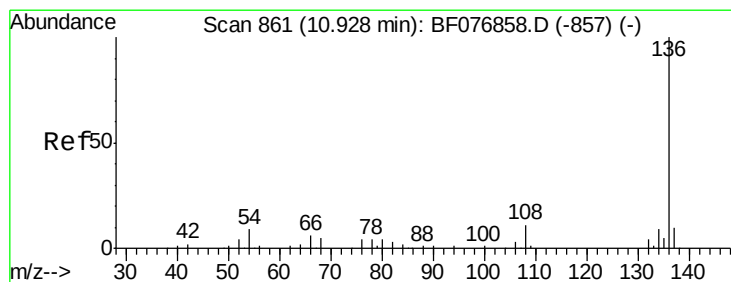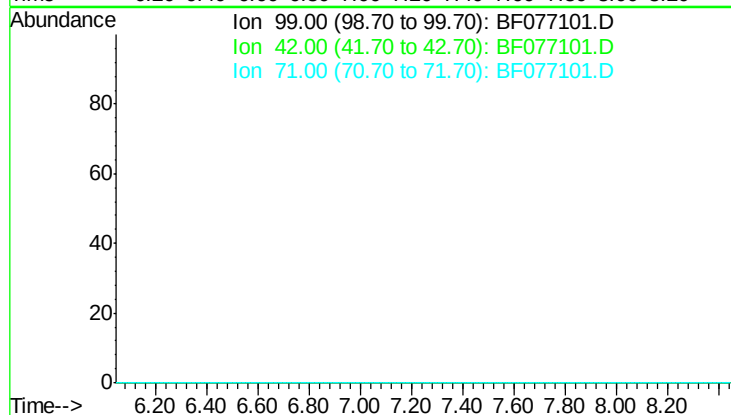

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 10.63 min Scan# 835

Delta R.T. -0.00 min

Lab File: BF077101.D

Acq: 28 Jan 2015 14:37

Tgt Ion:136 Resp: 88521



Ion Ratio Lower Upper

136 100

137 10.4 8.1 12.1

54 7.5 7.0 10.4

68 3.8 3.7 5.5

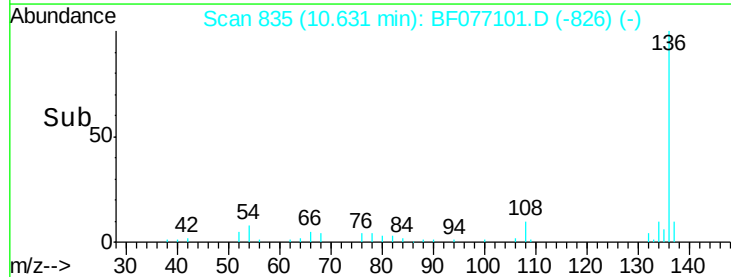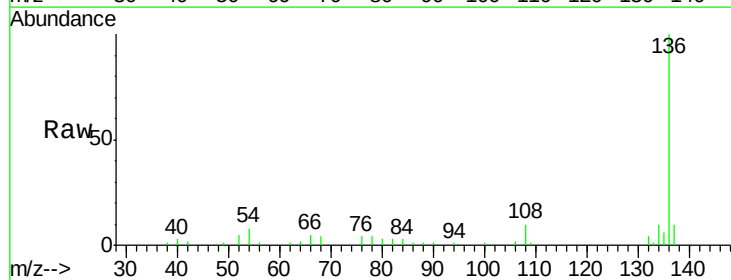



Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0

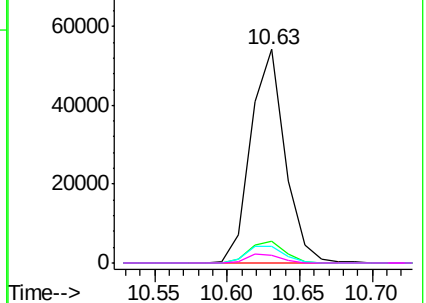


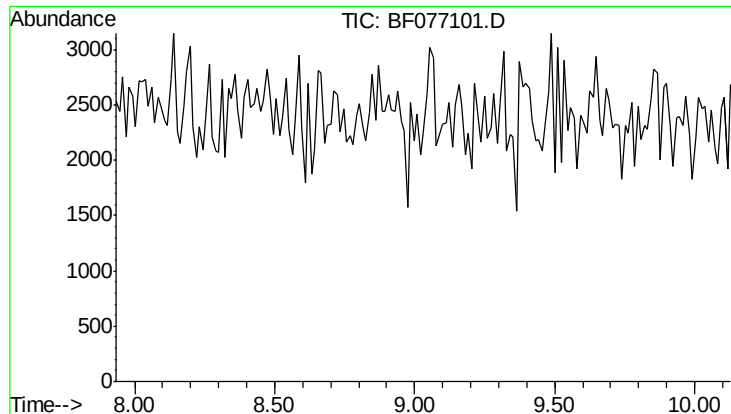


#23
 Nitrobenzene-d5
 Concen: 0.00 ng
 Expected RT: 9.03 min
 Lab File: BF077101.D
 Acq: 28 Jan 2015 14:37

Instrument :
 BNA_F
 ClientSampleId :
 SVOC-GPC-BLANK

Tgt Ion: 82




Sig	Exp Ratio
82	100
128	41.4
54	60.4

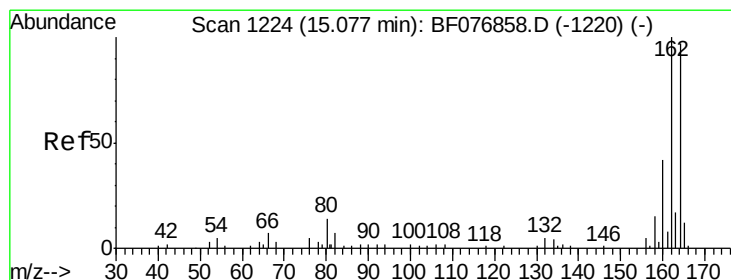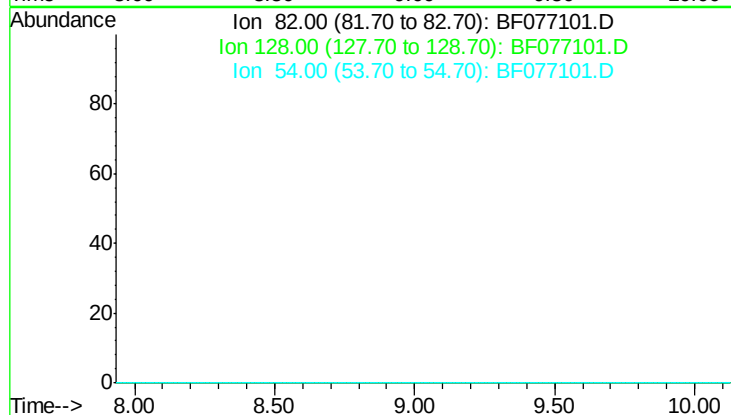


#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 14.75 min Scan# 1195
 Delta R.T. -0.01 min
 Lab File: BF077101.D
 Acq: 28 Jan 2015 14:37

Tgt Ion: 164 Resp: 48258

Ion	Ratio	Lower	Upper
164	100		
162	107.3	82.4	123.6
160	45.2	34.8	52.2

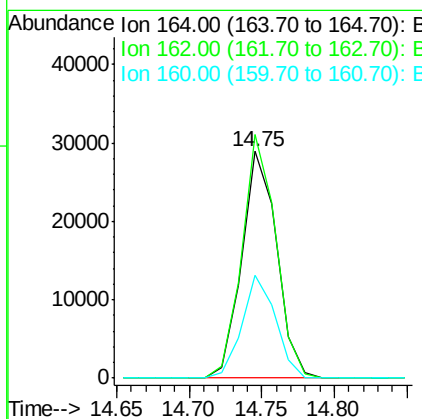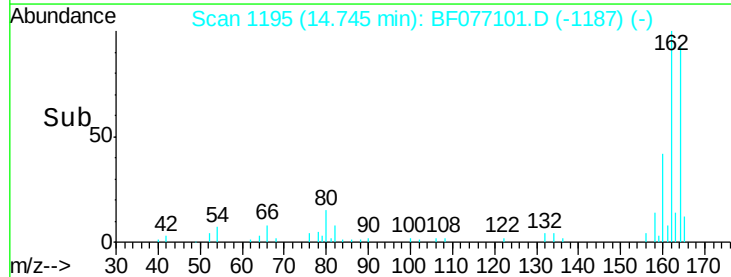
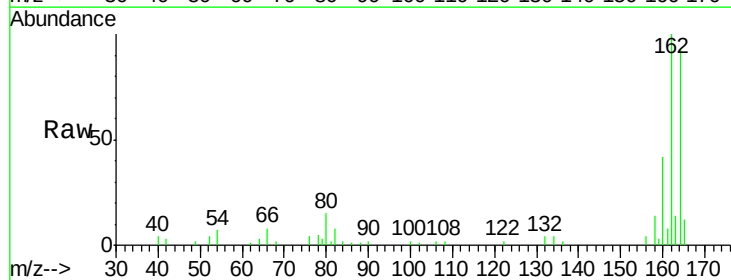


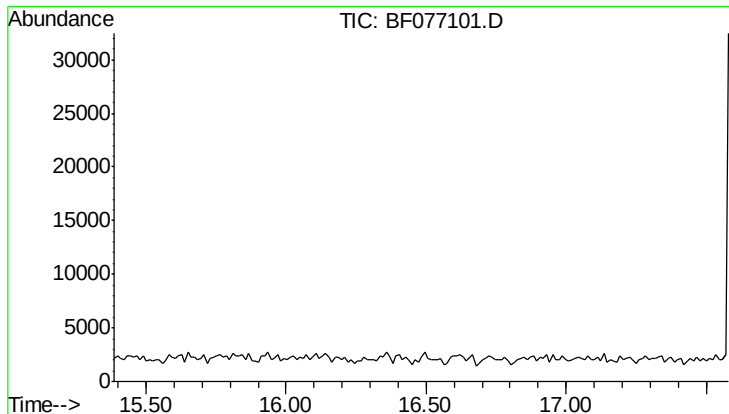

#41
 2,4,6-Tribromophenol
 Concen: 0.00 ng
 Expected RT: 16.48 min
 Lab File: BF077101.D
 Acq: 28 Jan 2015 14:37


Instrument :
 BNA_F
 ClientSampleId :
 SVOC-GPC-BLANK


Tgt Ion: 330
 Sig Exp Ratio
 330 100
 332 97.2
 141 48.1

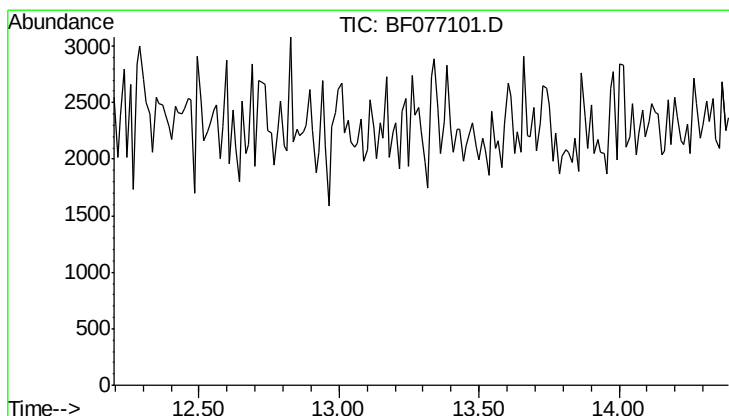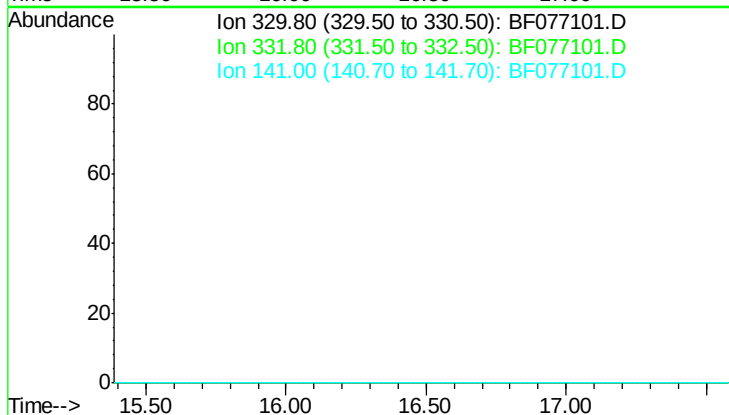

#44
 2-Fluorobiphenyl
 Concen: 0.00 ng
 Expected RT: 13.29 min
 Lab File: BF077101.D
 Acq: 28 Jan 2015 14:37

Tgt Ion: 172
 Sig Exp Ratio
 172 100
 171 33.3
 170 22.5

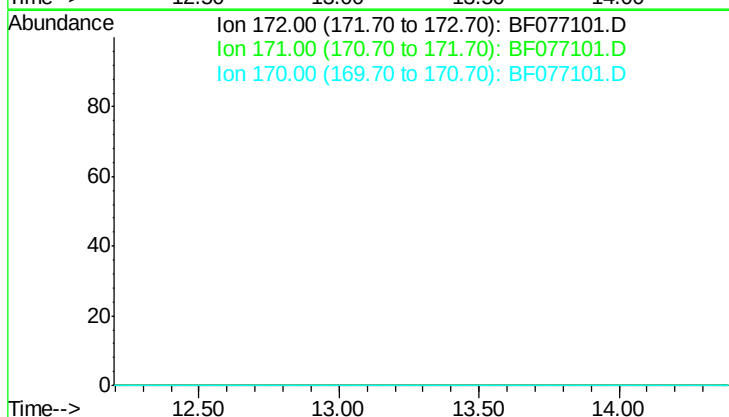

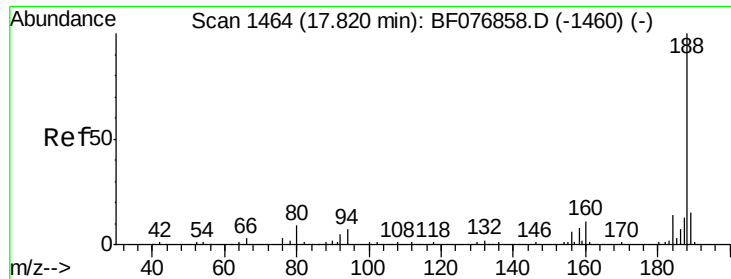

#63

Phenanthrene-d10

Concen: 20.00 ng

RT: 17.59 min Scan# 1444

Delta R.T. -0.01 min

Lab File: BF077101.D

Acq: 28 Jan 2015 14:37

Instrument :

BNA_F

ClientSampleId :

SVOC-GPC-BLANK


Tgt Ion:188 Resp: 80928

Ion Ratio Lower Upper

188 100

94 10.0 6.0 9.0#




80 9.8 6.9 10.3

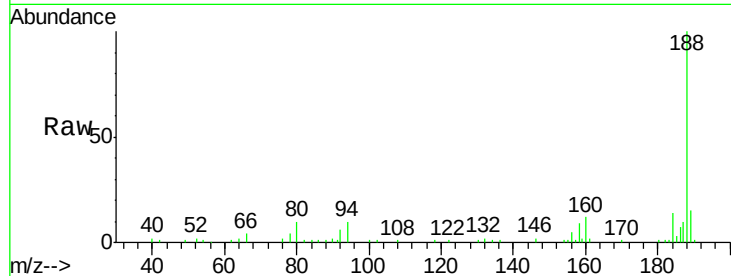

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF0

Ion 80.00 (79.70 to 80.70): BF0

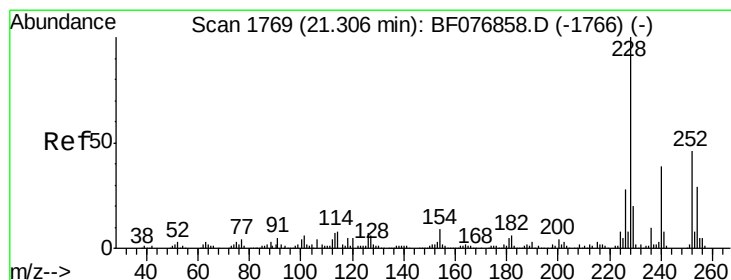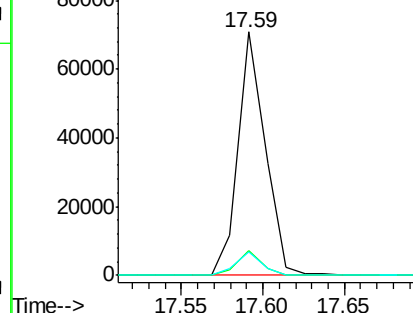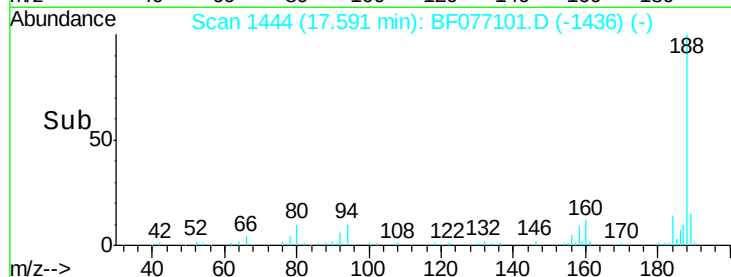

#75

Chrysene-d12

Concen: 20.00 ng

RT: 21.10 min Scan# 1751

Delta R.T. -0.01 min

Lab File: BF077101.D

Acq: 28 Jan 2015 14:37


Tgt Ion:240 Resp: 80147

Ion Ratio Lower Upper

240 100

120 8.8 10.4 15.6#



236 25.3 20.2 30.2

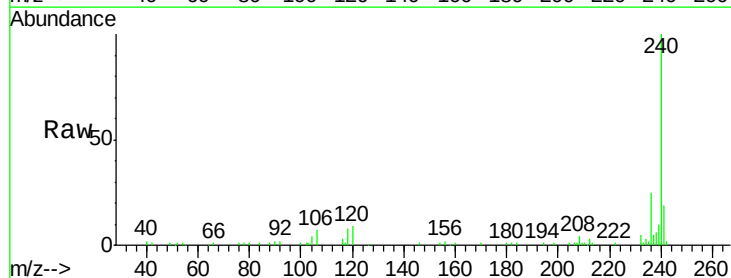


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

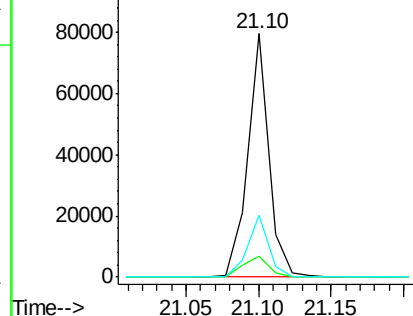
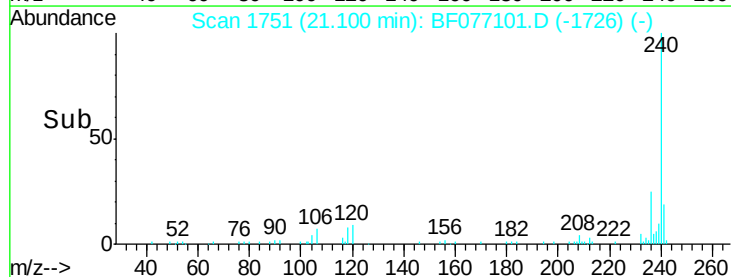


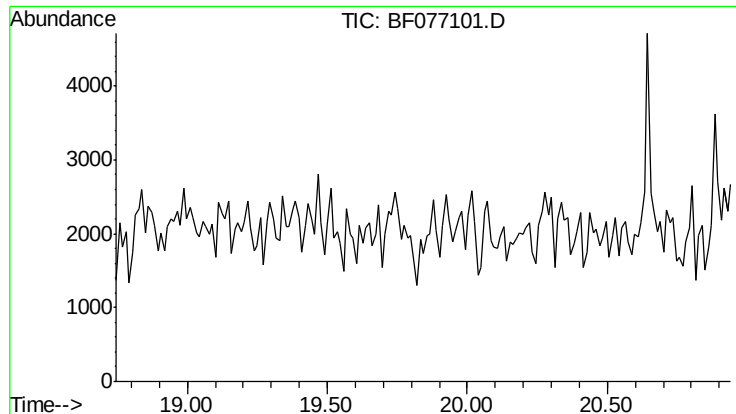

#78
 Terphenyl-d14
 Concen: 0.00 ng
 Expected RT: 19.84 min
 Lab File: BF077101.D
 Acq: 28 Jan 2015 14:37

Instrument :
 BNA_F
 ClientSampleId :
 SVOC-GPC-BLANK

Tgt Ion: 244
 Sig Exp Ratio
 244 100
 212 7.9
 122 12.6

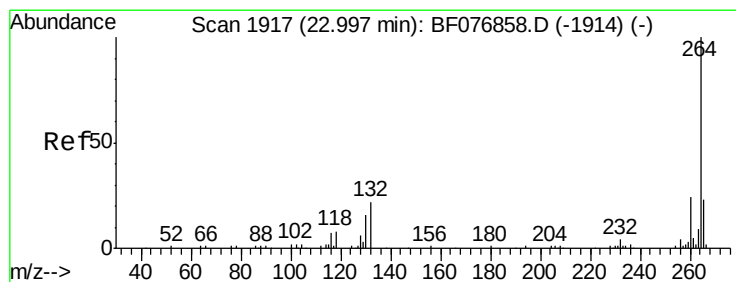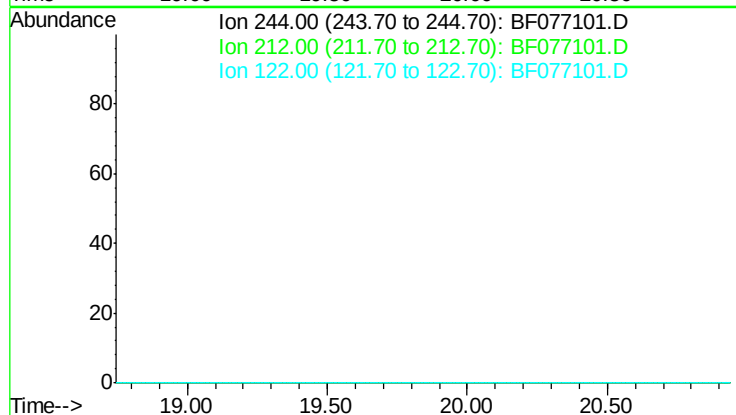

#86
 Perylene-d12
 Concen: 20.00 ng
 RT: 22.75 min Scan# 1895
 Delta R.T. -0.07 min
 Lab File: BF077101.D
 Acq: 28 Jan 2015 14:37

Tgt Ion: 264 Resp: 73579
 Ion Ratio Lower Upper
 264 100
 260 24.1 19.0 28.4
 265 22.1 18.1 27.1

