

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF012815\
 Data File : BF077101.D
 Acq On : 28 Jan 2015 14:37
 Operator : TP/IZ
 Sample : G1175-05
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SVOC-GPC-BLANK

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF011415.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.384	25	26	38	rBV	49024	125471	62.62%	8.281%
2	1.635	47	48	52	rBV3	904	2079	1.04%	0.137%
3	1.864	64	68	70	rBV2	879	2215	1.11%	0.146%
4	2.173	92	95	99	rVB2	965	2687	1.34%	0.177%
5	2.298	104	106	110	rVB3	1205	2713	1.35%	0.179%
6	2.378	112	113	117	rVV2	1370	2212	1.10%	0.146%
7	2.470	120	121	125	rVB2	1017	2172	1.08%	0.143%
8	2.721	141	143	146	rVB2	1026	2243	1.12%	0.148%
9	2.984	163	166	168	rBV2	865	2381	1.19%	0.157%
10	3.121	175	178	180	rVB2	967	2223	1.11%	0.147%
11	3.384	197	201	203	rBV2	1057	2531	1.26%	0.167%
12	4.241	273	276	279	rBV2	1196	2086	1.04%	0.138%
13	4.356	283	286	290	rVB3	818	2180	1.09%	0.144%
14	5.407	376	378	383	rVB2	1334	2993	1.49%	0.198%
15	5.556	390	391	394	rBV	1078	2458	1.23%	0.162%
16	5.682	399	402	405	rBV2	1373	2646	1.32%	0.175%
17	5.933	419	424	426	rVB2	1244	3395	1.69%	0.224%
18	6.024	428	432	434	rVB	956	2479	1.24%	0.164%
19	6.230	446	450	452	rBV2	1285	2414	1.20%	0.159%
20	6.573	476	480	482	rVB4	1040	2649	1.32%	0.175%
21	6.619	482	484	489	rBV3	1033	2818	1.41%	0.186%
22	7.316	541	545	549	rVB2	938	2289	1.14%	0.151%
23	7.613	568	571	575	rVB2	998	2490	1.24%	0.164%
24	7.716	577	580	585	rVB	77272	124379	62.08%	8.209%
25	10.185	793	796	799	rBV	825	2824	1.41%	0.186%
26	10.436	815	818	821	rVB3	989	2311	1.15%	0.153%
27	10.631	831	835	839	rBV	104782	170326	85.01%	11.241%
28	10.928	860	861	865	rBV	1233	2238	1.12%	0.148%
29	11.419	903	904	908	rVB2	1097	2147	1.07%	0.142%
30	11.842	939	941	946	rVB2	1200	2787	1.39%	0.184%
31	12.174	965	970	973	rBV3	1232	4197	2.09%	0.277%
32	12.288	978	980	984	rBV3	1272	3519	1.76%	0.232%
33	13.008	1039	1043	1047	rBV4	1089	4195	2.09%	0.277%
34	13.259	1064	1065	1070	rVB2	995	2105	1.05%	0.139%

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF012815\
 Data File : BF077101.D
 Acq On : 28 Jan 2015 14:37
 Operator : TP/IZ
 Sample : G1175-05
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SVOC-GPC-BLANK

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF011415.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	13.339	1070	1072	1074	rBV2	1138	2141	1.07%	0.141%
36	13.728	1104	1106	1111	rVB2	782	2123	1.06%	0.140%
37	14.745	1192	1195	1199	rBV	118481	189391	94.53%	12.499%
38	14.814	1199	1201	1206	rVB	4926	10562	5.27%	0.697%
39	15.088	1222	1225	1228	rVB	1583	3588	1.79%	0.237%
40	15.763	1280	1284	1287	rBV3	886	3185	1.59%	0.210%
41	16.357	1333	1336	1338	rVB2	1096	2261	1.13%	0.149%
42	16.494	1344	1348	1350	rBV	1192	2643	1.32%	0.174%
43	16.723	1364	1368	1370	rBV2	928	2512	1.25%	0.166%
44	17.591	1441	1444	1447	rBV	174284	194966	97.31%	12.867%
45	18.391	1510	1514	1515	rVB2	961	2185	1.09%	0.144%
46	18.837	1549	1553	1554	rBV2	1267	2943	1.47%	0.194%
47	19.740	1628	1632	1634	rBV2	1034	2880	1.44%	0.190%
48	20.072	1658	1661	1664	rBV	996	2180	1.09%	0.144%
49	20.220	1667	1674	1676	rVB2	592	2203	1.10%	0.145%
50	20.334	1682	1684	1687	rBV3	892	2109	1.05%	0.139%
51	20.643	1706	1711	1716	rBV3	3003	4842	2.42%	0.320%
52	20.883	1729	1732	1734	rBV2	2128	3396	1.69%	0.224%
53	21.066	1746	1748	1749	rBV2	2998	4143	2.07%	0.273%
54	21.100	1749	1751	1754	rVV	195689	200354	100.00%	13.223%
55	21.329	1768	1771	1775	rBV2	837	2125	1.06%	0.140%
56	21.580	1788	1793	1796	rBV3	1220	4330	2.16%	0.286%
57	21.683	1798	1802	1809	rVV4	4090	7764	3.88%	0.512%
58	21.889	1819	1820	1825	rVB	1068	2212	1.10%	0.146%
59	22.358	1857	1861	1863	rBV3	1541	3995	1.99%	0.264%
60	22.586	1878	1881	1883	rBV2	931	2422	1.21%	0.160%
61	22.632	1883	1885	1888	rVB2	2285	3625	1.81%	0.239%
62	22.746	1892	1895	1898	rBV	161341	188356	94.01%	12.431%
63	22.883	1904	1907	1911	rVB2	2221	5601	2.80%	0.370%
64	22.986	1911	1916	1917	rBV4	3624	8296	4.14%	0.548%
65	23.009	1917	1918	1922	rVB3	2596	5081	2.54%	0.335%
66	23.066	1922	1923	1924	rBV	2197	2296	1.15%	0.152%
67	23.100	1924	1926	1929	rVB3	980	2529	1.26%	0.167%
68	23.203	1934	1935	1936	rVV	2705	2751	1.37%	0.182%
69	23.283	1939	1942	1943	rVV2	2252	3929	1.96%	0.259%
70	23.352	1945	1948	1951	rVB4	4149	7771	3.88%	0.513%
71	23.409	1951	1953	1955	rBV2	2022	3595	1.79%	0.237%

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF012815\
 Data File : BF077101.D
 Acq On : 28 Jan 2015 14:37
 Operator : TP/IZ
 Sample : G1175-05
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SVOC-GPC-BLANK

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF011415.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

72	23.649	1972	1974	1975	rBV2	1746	2446	1.22%	0.161%
73	23.706	1975	1979	1984	rVV6	3491	9597	4.79%	0.633%
74	24.083	2010	2012	2016	rBV4	2597	5245	2.62%	0.346%
75	24.198	2020	2022	2024	rBV3	1897	2921	1.46%	0.193%
76	24.266	2024	2028	2029	rBV4	1627	4183	2.09%	0.276%
77	24.358	2033	2036	2037	rBV3	3043	6081	3.04%	0.401%
78	24.392	2037	2039	2041	rVB3	2618	3486	1.74%	0.230%
79	24.495	2047	2048	2051	rBV2	2318	4300	2.15%	0.284%
80	24.563	2052	2054	2055	rVB2	2579	2883	1.44%	0.190%
81	24.598	2055	2057	2058	rBV	2611	3371	1.68%	0.222%
82	24.849	2074	2079	2085	rBV8	2898	12773	6.38%	0.843%
83	24.941	2085	2087	2090	rBV3	1581	3637	1.82%	0.240%
84	24.998	2090	2092	2094	rVV3	1463	2391	1.19%	0.158%
85	25.055	2096	2097	2100	rVB2	2666	4299	2.15%	0.284%
86	25.135	2103	2104	2107	rBV3	2047	3495	1.74%	0.231%
87	25.672	2149	2151	2153	rVB2	2385	3597	1.80%	0.237%
88	25.809	2161	2163	2166	rVB4	2133	3775	1.88%	0.249%
89	25.992	2177	2179	2180	rBV	1445	2326	1.16%	0.154%
90	26.152	2192	2193	2196	rBV3	1736	2486	1.24%	0.164%
91	26.244	2200	2201	2204	rBV3	2642	5597	2.79%	0.369%
92	26.369	2210	2212	2214	rBV3	1909	2094	1.05%	0.138%
93	26.472	2219	2221	2224	rBV4	2632	4877	2.43%	0.322%
94	26.575	2229	2230	2232	rBV	2553	2815	1.41%	0.186%
95	26.678	2236	2239	2240	rBV3	1817	3559	1.78%	0.235%
96	26.758	2245	2246	2249	rVB3	1658	3122	1.56%	0.206%
97	26.827	2250	2252	2254	rBV2	1808	2911	1.45%	0.192%
98	27.169	2280	2282	2285	rVB4	1547	2620	1.31%	0.173%
99	27.238	2286	2288	2290	rBV3	1890	2744	1.37%	0.181%
100	27.295	2291	2293	2295	rVB3	2506	3440	1.72%	0.227%


Sum of corrected areas: 1515208

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF012815\
Data File : BF077101.D
Acq On : 28 Jan 2015 14:37
Operator : TP/IZ
Sample : G1175-05
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SVOC-GPC-BLANK

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF011415.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

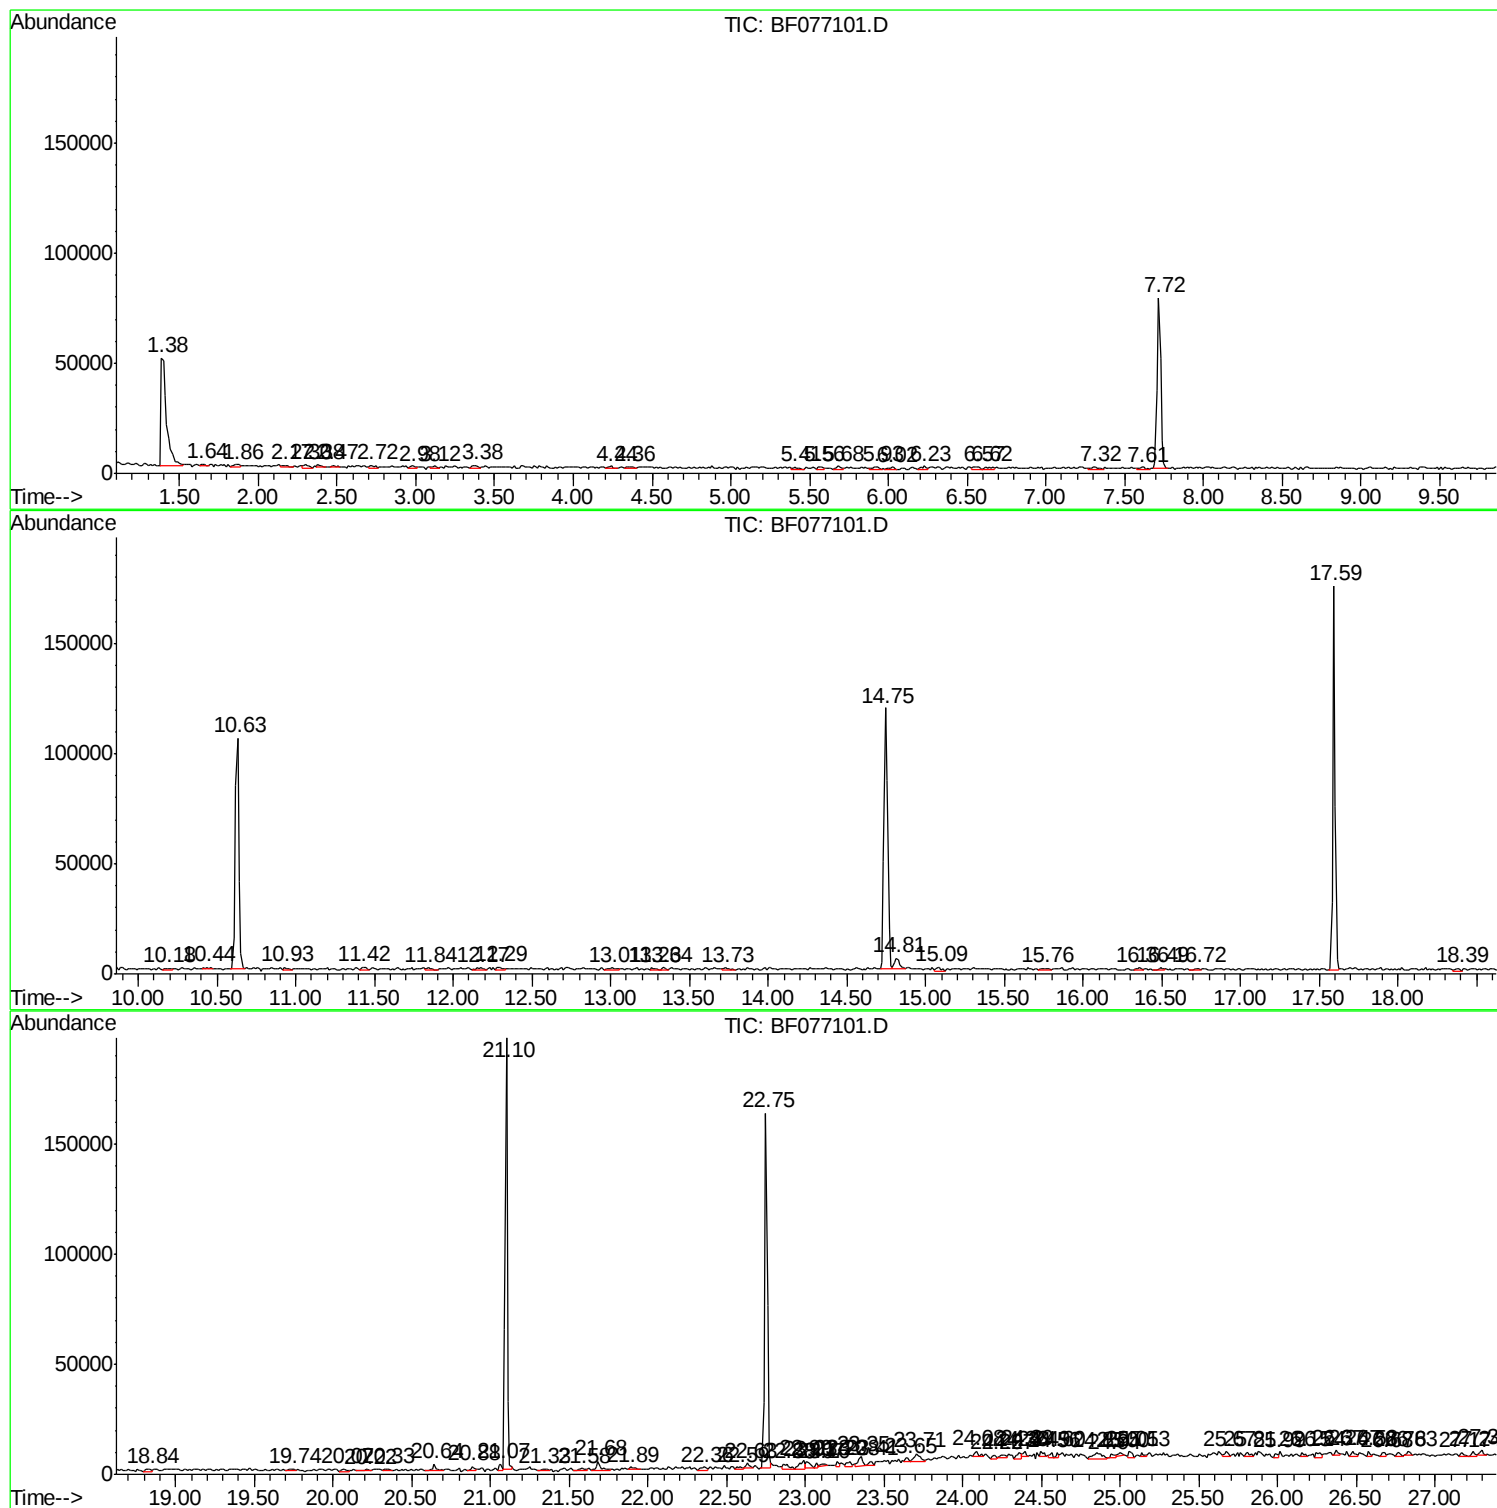

DbaaaPathh::ZZ\NRPBHHM1BBAFNDAAABBB0028855\
 DbaaaFile::BB0071001DD
 Aeqq00n ::288Jan20055 144337
 Oppaaaor ::TPPIZZ
 Saaapbe ::G01735005
 MMscc ::
 AASSVaal ::55 SaaapbeMMuippler:11

Instrument :
 BNA_F
 ClientSampleId :
 SVOC-GPC-BLANK

QqaabtMebbdd::ZZ\NRPBHHM1BBAFMEH00BS8270BB0014455MM
 QqaabtTife ::ASBPBBAASSANDBBSF00R55P000NTC6AIBBATION

TICCLibbaay ::CC\DAABASSEN0\$S002LL
 TICInteggaionPaaameess:LS6CNTTP

TIC Top Hit name	RT	EstConc	Units	Response	-Internal Standard-	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---------------------	---	----	------	------

No Library Search Compounds Detected
