


Data Path : Z:\HPCHEM1\BNA_F\Data\BF012815\
 Data File : BF077097.D
 Acq On : 28 Jan 2015 11:50
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF011415.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jan 28 16:07:35 2015

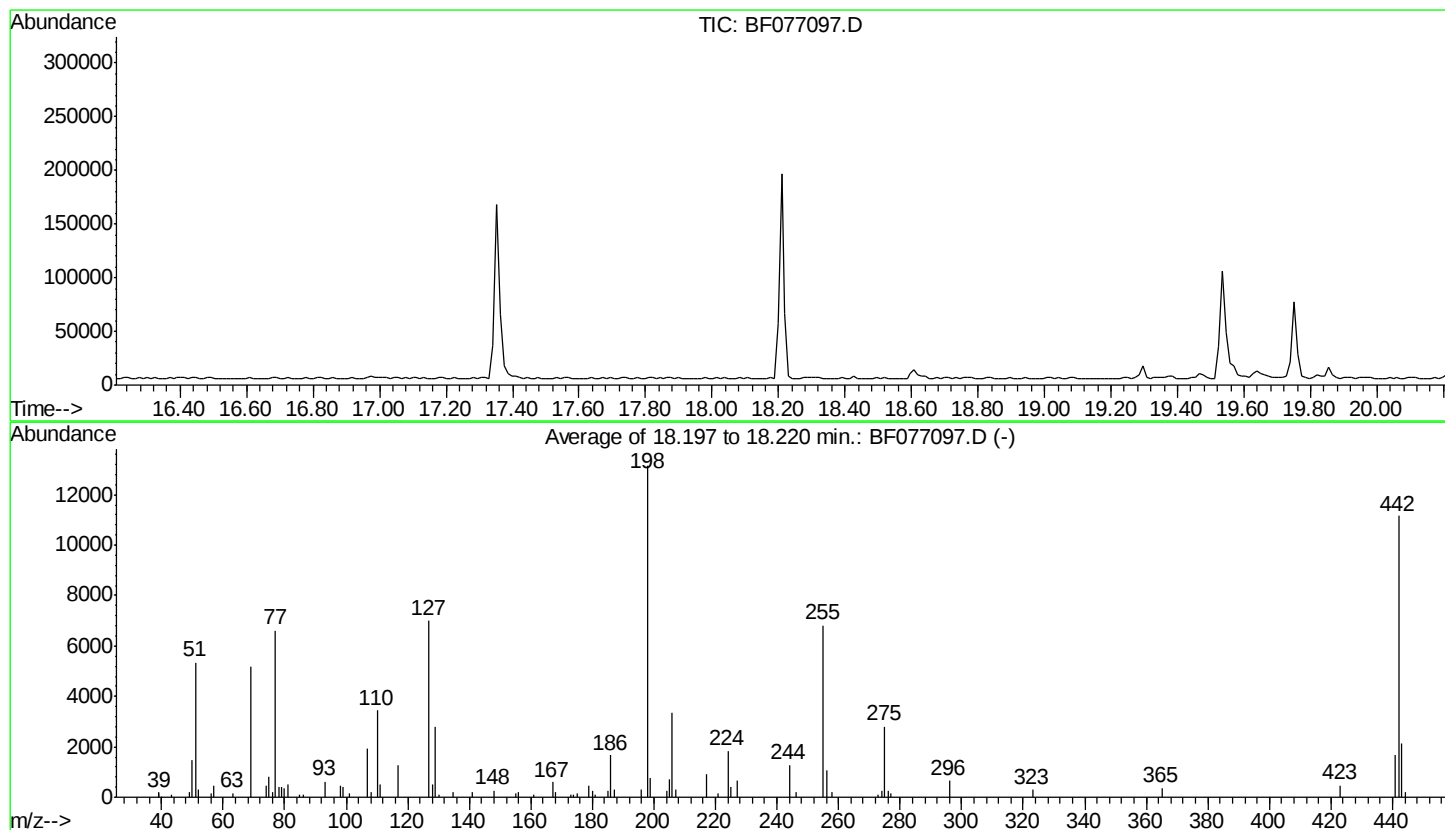

AutoFind: Scans 1497, 1498, 1499; Background Corrected with Scan 1494

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.6	5338	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	39.4	5178	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	53.2	7004	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	13154	PASS
199	198	5	9	6.0	786	PASS
275	198	10	60	21.3	2806	PASS
365	198	1	100	2.7	359	PASS
441	442	0.01	24	14.8	1654	PASS
442	198	50	100	84.8	11155	PASS
443	442	15	24	19.0	2114	PASS