


Data Path : Z:\HPCHEM1\BNA_F\Data\BF012815\
 Data File : BF077115.D
 Acq On : 29 Jan 2015 2:08
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF011415.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jan 28 16:07:35 2015

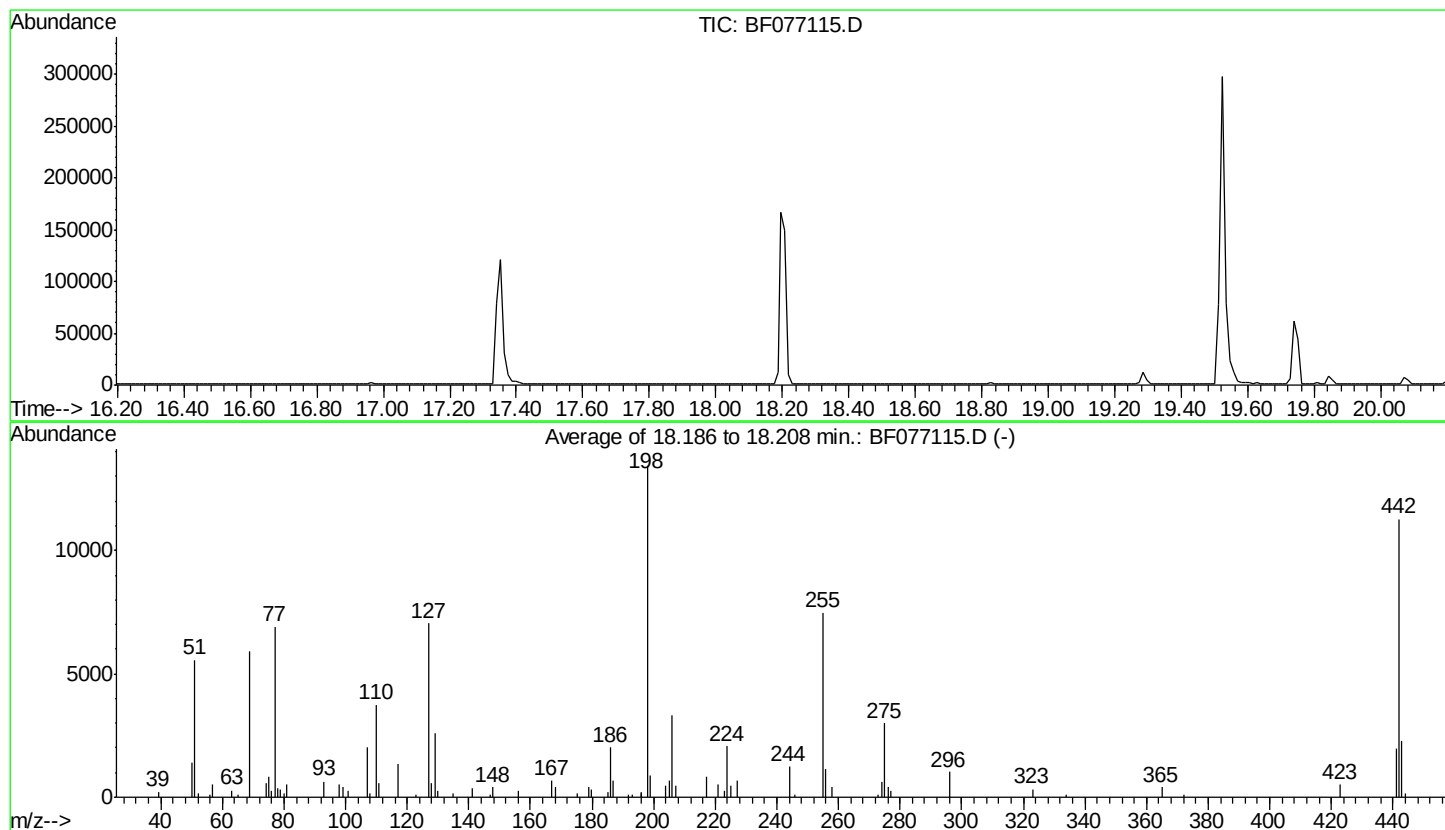

AutoFind: Scans 1496, 1497, 1498; Background Corrected with Scan 1493

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.3	5553	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	44.0	5911	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	52.4	7048	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	13441	PASS
199	198	5	9	6.6	887	PASS
275	198	10	60	22.3	2995	PASS
365	198	1	100	3.0	407	PASS
441	442	0.01	24	17.6	1985	PASS
442	198	50	100	83.8	11266	PASS
443	442	15	24	20.1	2268	PASS