


Data Path : Z:\HPCHEM1\BNA F\Data\BF012818\
 Data File : BF102554.D
 Acq On : 28 Jan 2018 13:46
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF012218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Jan 27 20:48:40 2018

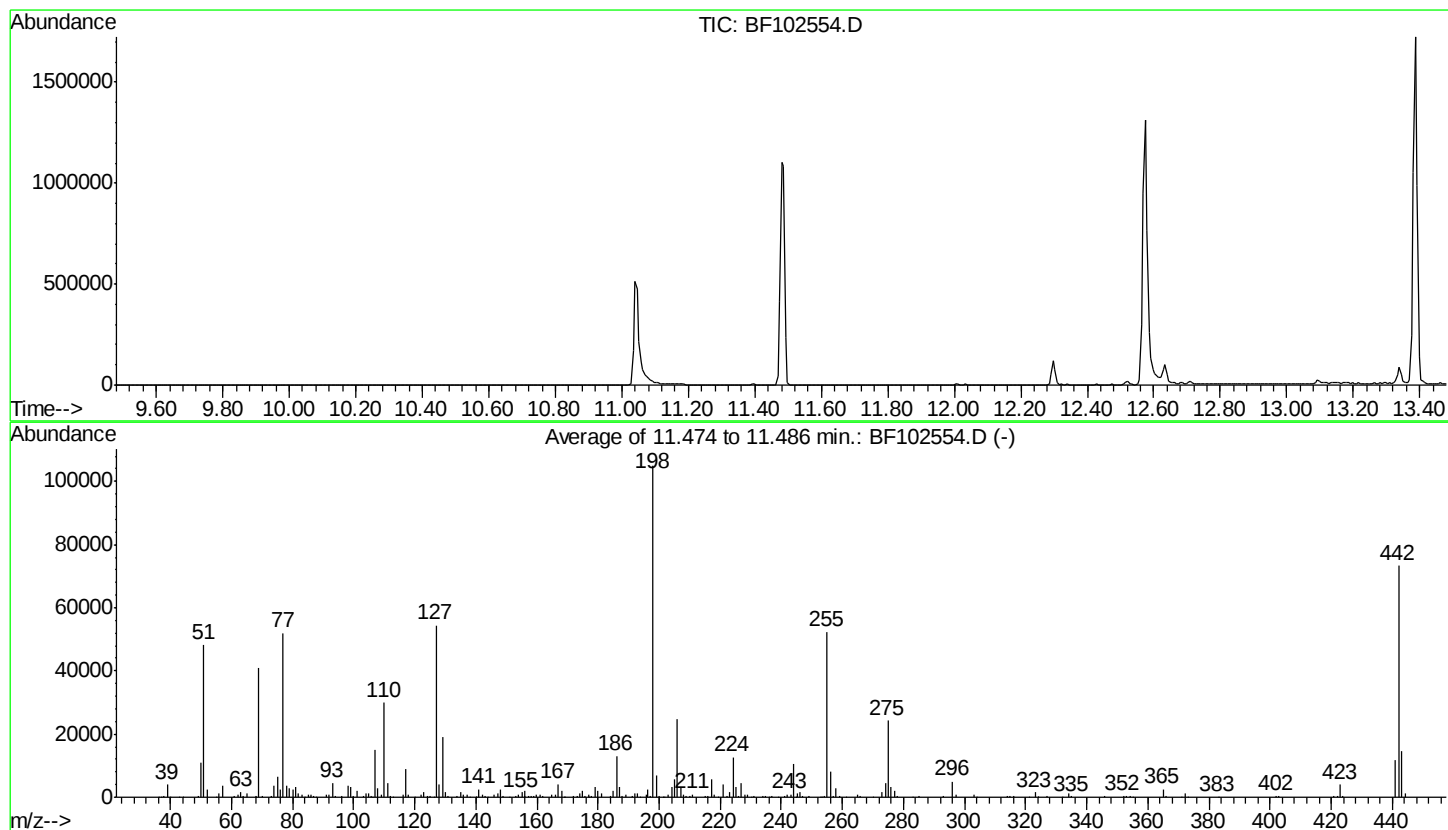

AutoFind: Scans 1596, 1597, 1598; Background Corrected with Scan 1592

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.0	48336	PASS
68	69	0.00	2	1.5	623	PASS
69	198	0.00	100	38.9	40805	PASS
70	69	0.00	2	0.7	287	PASS
127	198	10	80	51.9	54472	PASS
197	198	0.00	2	0.6	587	PASS
198	198	100	100	100.0	105002	PASS
199	198	5	9	6.5	6774	PASS
275	198	10	60	23.0	24149	PASS
365	198	1	100	2.4	2558	PASS
441	443	0.01	100	80.3	11774	PASS
442	198	50	100	69.8	73253	PASS
443	442	15	24	20.0	14671	PASS