


Data Path : Z:\HPCHEM1\BNA F\Data\BF012818\
 Data File : BF102581.D
 Acq On : 29 Jan 2018 2:53
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF012218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Jan 27 20:48:40 2018

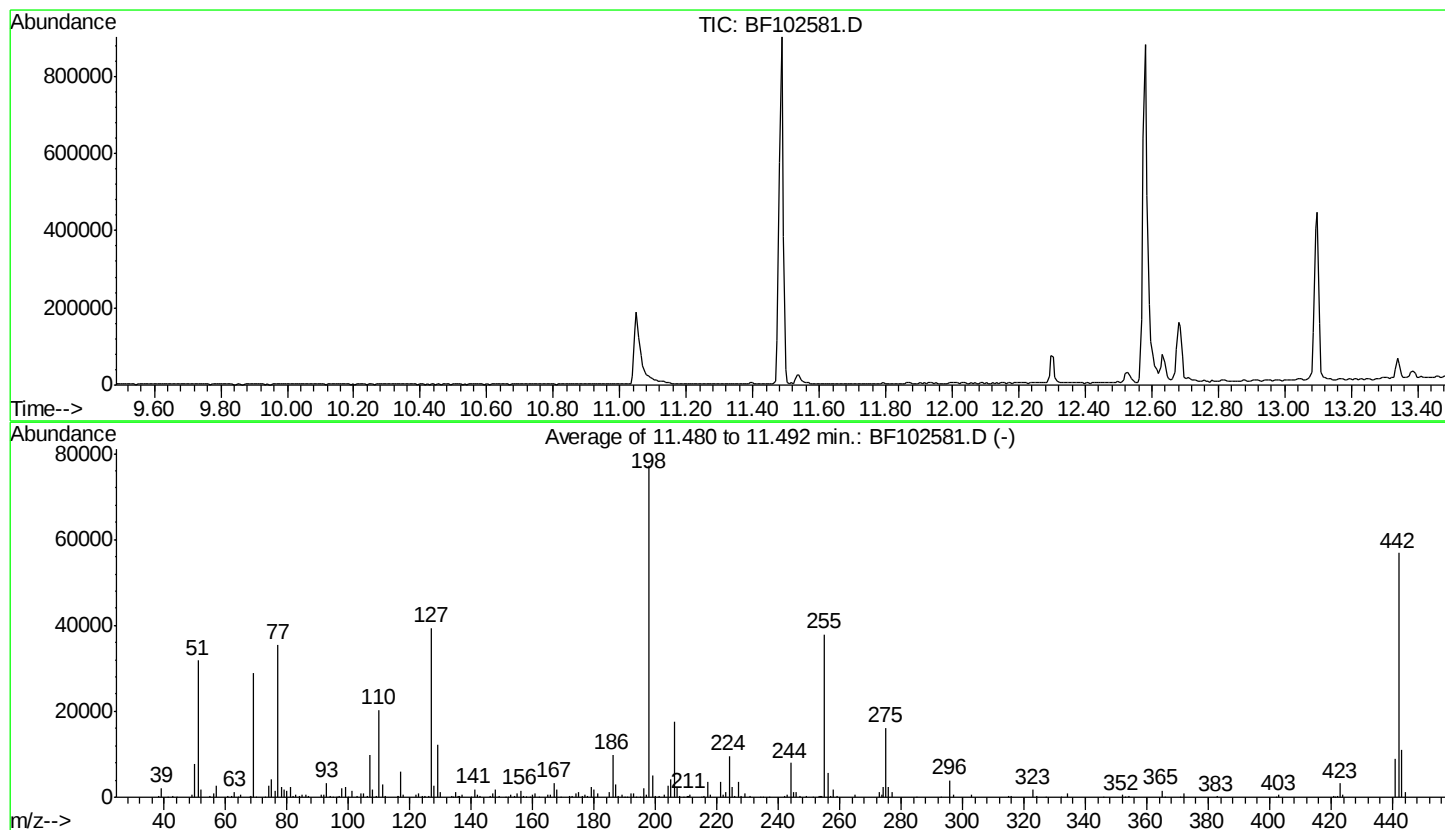

AutoFind: Scans 1597, 1598, 1599; Background Corrected with Scan 1592

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.2	31765	PASS
68	69	0.00	2	1.4	394	PASS
69	198	0.00	100	37.4	28839	PASS
70	69	0.00	2	0.5	157	PASS
127	198	10	80	51.0	39352	PASS
197	198	0.00	2	0.6	465	PASS
198	198	100	100	100.0	77186	PASS
199	198	5	9	6.5	5040	PASS
275	198	10	60	21.0	16217	PASS
365	198	1	100	2.0	1553	PASS
441	443	0.01	100	82.0	9009	PASS
442	198	50	100	73.6	56773	PASS
443	442	15	24	19.4	10991	PASS