
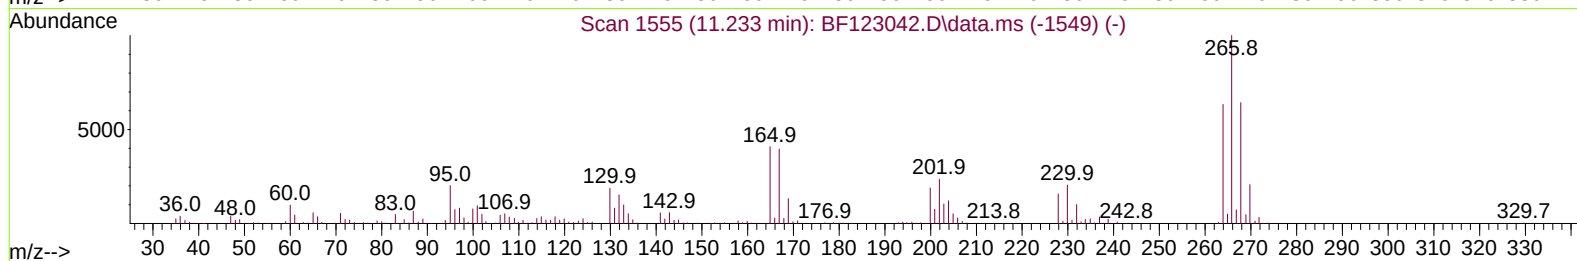
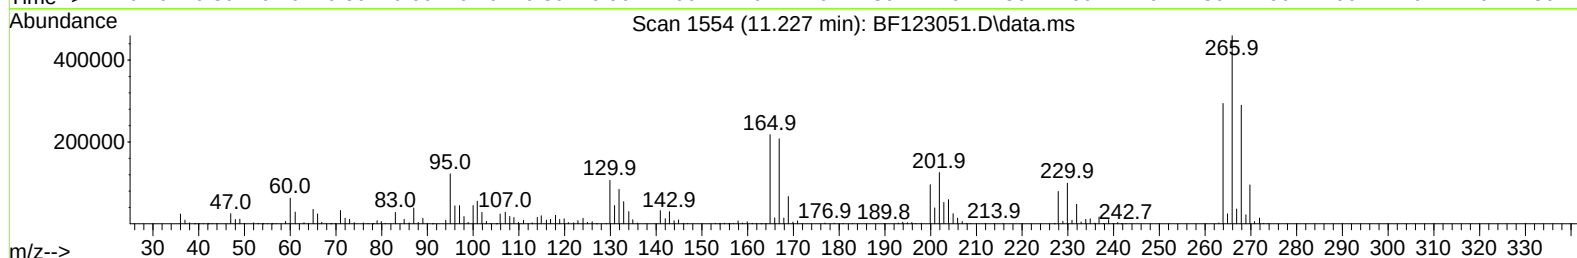


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012821\
 Data File : BF123051.D
 Acq On : 28 Jan 2021 9:43
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 29 03:11:02 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jan 28 00:48:07 2021
 Response via : Initial Calibration

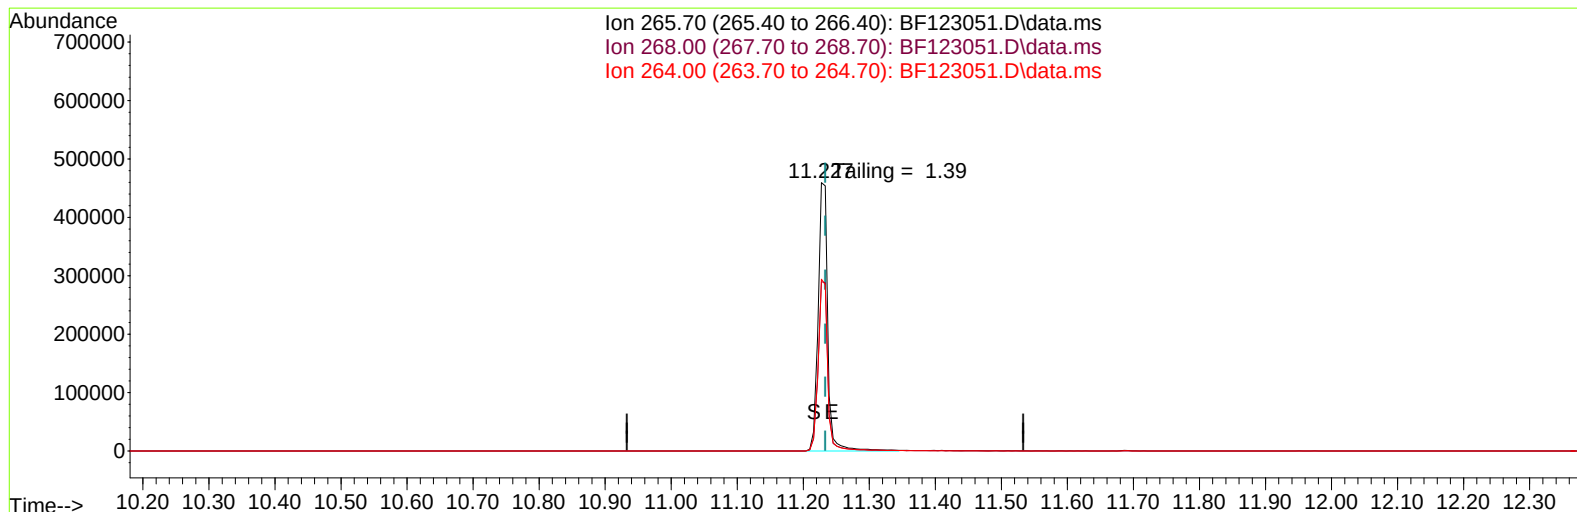




TIC: BF123051.D\data.ms

(70) Pentachlorophenol (C)**11.227min (-0.006) 38031.38 ng****response 470192**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	63.11
264.00	62.30	64.02
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012821\
 Data File : BF123051.D
 Acq On : 28 Jan 2021 9:43
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 29 03:11:02 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jan 28 00:48:07 2021
 Response via : Initial Calibration

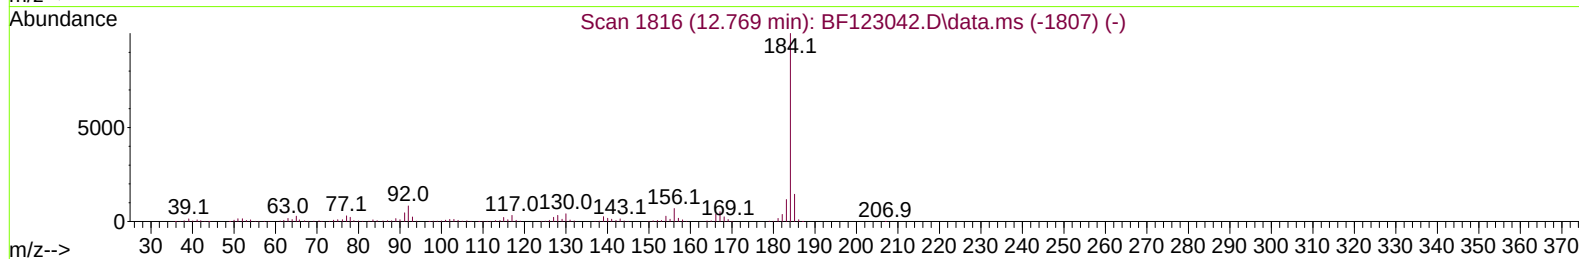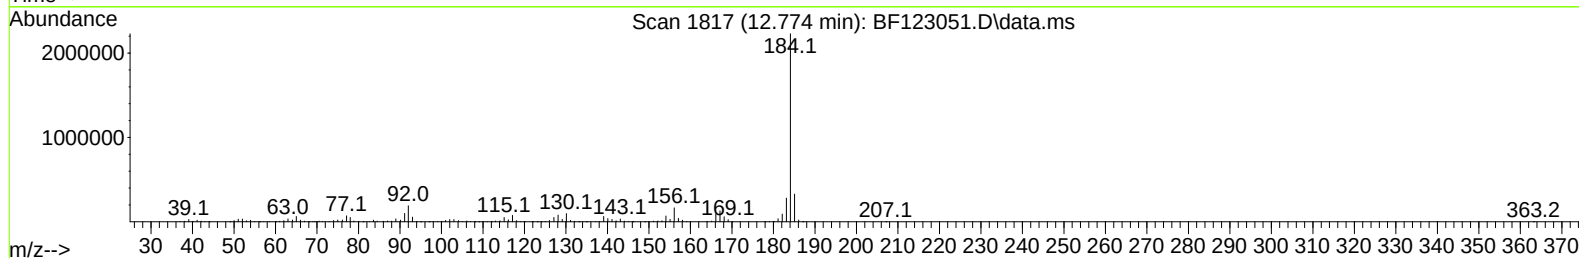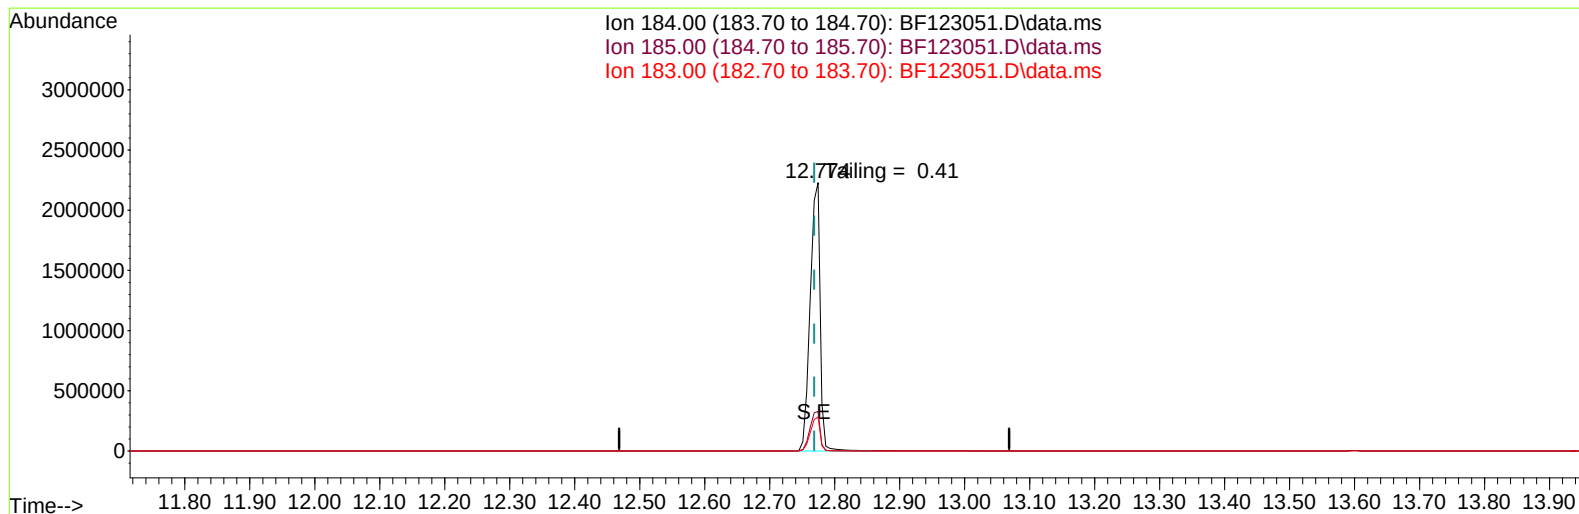

TIC: BF123051.D\data.ms

(77) Benzidine

12.774min (+ 0.006) 0.00 ng

response 2389726

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.72
183.00	12.10	12.61
0.00	0.00	0.00