

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012821\
 Data File : BF123055.D
 Acq On : 28 Jan 2021 12:01
 Operator : JU/CG
 Sample : PB134374BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB134374BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012721.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF123055.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.522	578	584	587	rBV	6733396	7243570	71.77%	12.094%
2	6.516	747	753	756	rBV	6207045	7237075	71.70%	12.083%
3	6.892	813	817	820	rBV	2224667	1781457	17.65%	2.974%
4	7.451	906	912	915	rBV	4507130	4883727	48.39%	8.154%
5	8.175	1030	1035	1038	rBV	2452027	2429822	24.07%	4.057%
6	9.251	1212	1218	1222	rBV	7111445	8676655	85.96%	14.487%
7	9.933	1328	1334	1338	rBV	2962286	2904285	28.77%	4.849%
8	10.727	1462	1469	1472	rBV	5408001	5787715	57.34%	9.663%
9	11.427	1582	1588	1591	rBV	3192692	2989756	29.62%	4.992%
10	13.027	1852	1860	1863	rBV	9098146	10093456	100.00%	16.852%
11	14.074	2034	2038	2042	rBV	3179998	2991560	29.64%	4.995%
12	15.562	2282	2291	2296	rBV	2252250	2875150	28.49%	4.800%




Sum of corrected areas: 59894228

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012821\
Data File : BF123055.D
Acq On : 28 Jan 2021 12:01
Operator : JU/CG
Sample : PB134374BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB134374BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

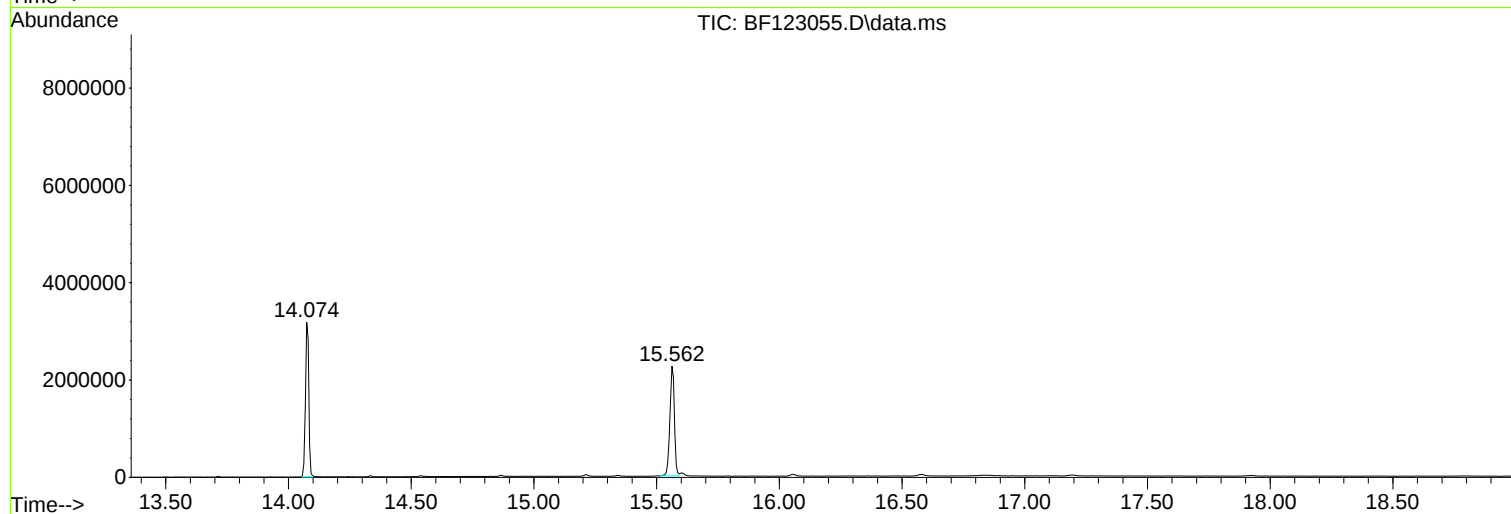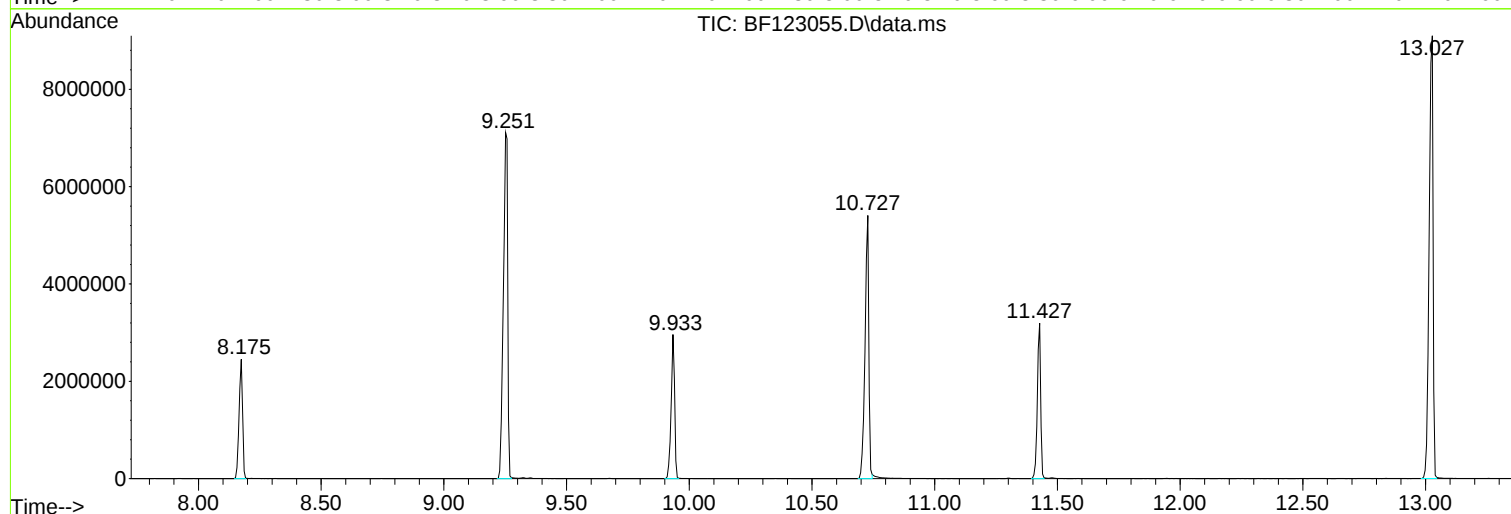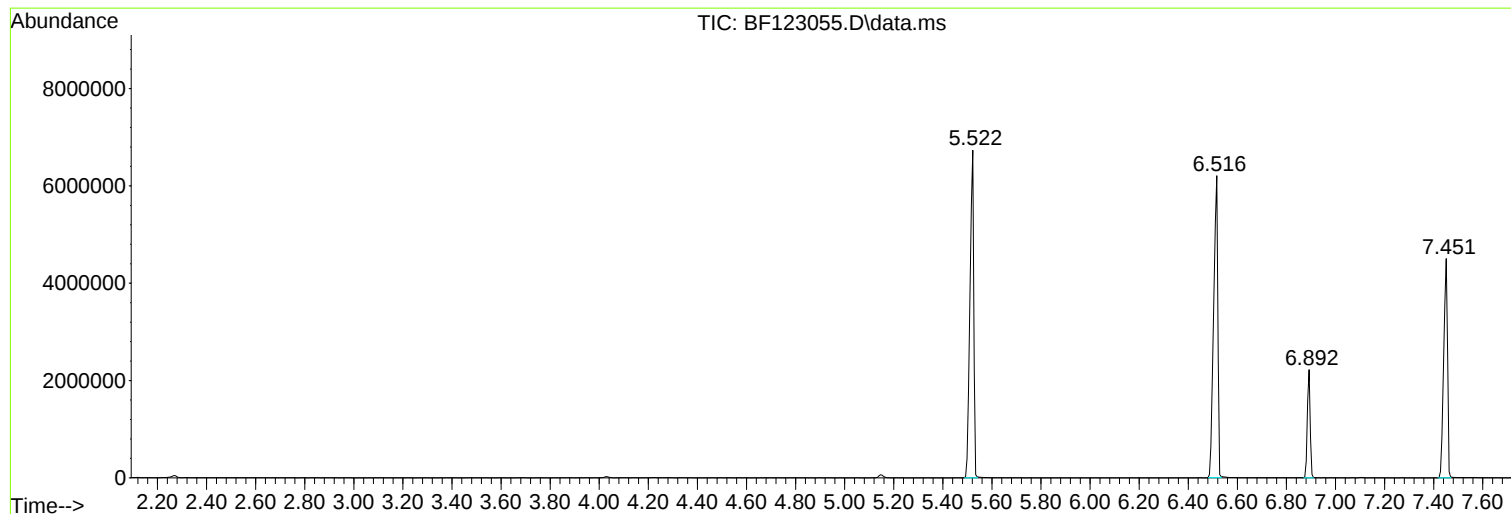

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012821\
Data File : BF123055.D
Acq On : 28 Jan 2021 12:01
Operator : JU/CG
Sample : PB134374BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB134374BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012821\
Data File : BF123055.D
Acq On : 28 Jan 2021 12:01
Operator : JU/CG
Sample : PB134374BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB134374BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------