
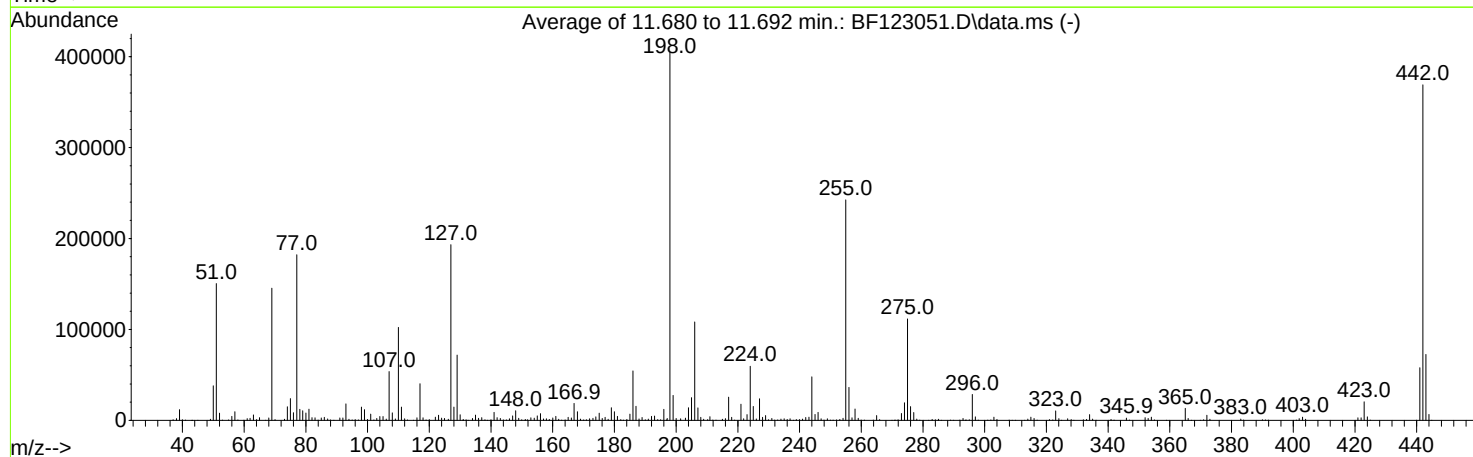


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012821\
 Data File : BF123051.D
 Acq On : 28 Jan 2021 9:43
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012721.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jan 28 00:48:07 2021

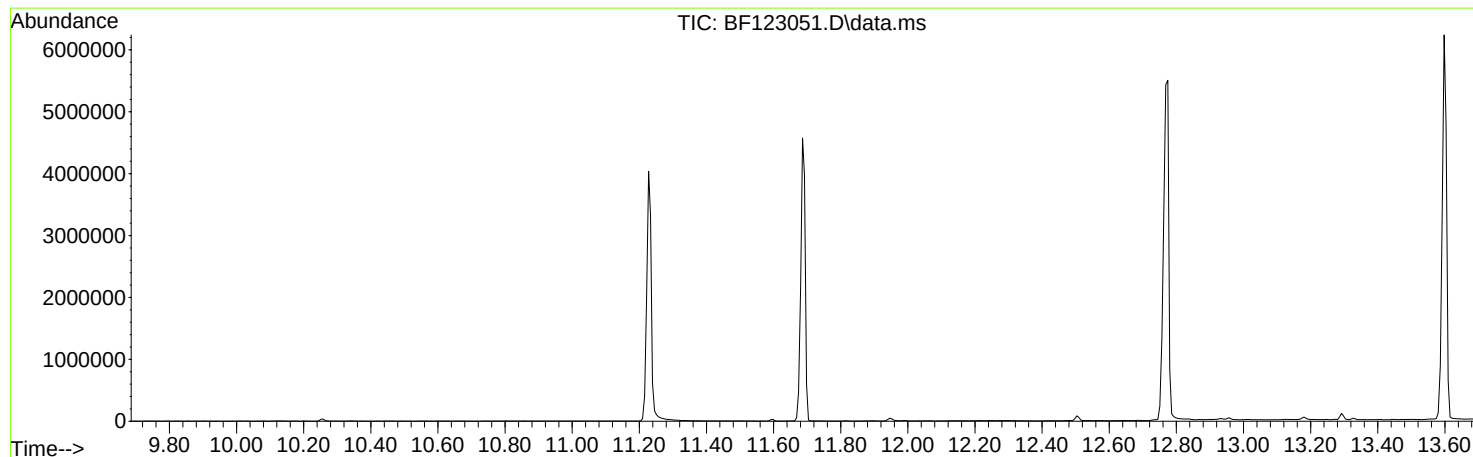

AutoFind: Scans 1631, 1632, 1633; Background Corrected with Scan 1625

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.2	150520	PASS
68	69	0.00	2	1.9	2702	PASS
69	198	0.00	100	35.9	145299	PASS
70	69	0.00	2	0.6	843	PASS
127	198	10	80	47.8	193323	PASS
197	198	0.00	2	0.5	2110	PASS
198	198	100	100	100.0	404629	PASS
199	198	5	9	6.8	27376	PASS
275	198	10	60	27.6	111515	PASS
365	198	1	100	3.3	13157	PASS
441	198	0.01	100	14.3	57965	PASS
442	442	50	100	100.0	369024	PASS
443	442	15	24	19.7	72563	PASS