
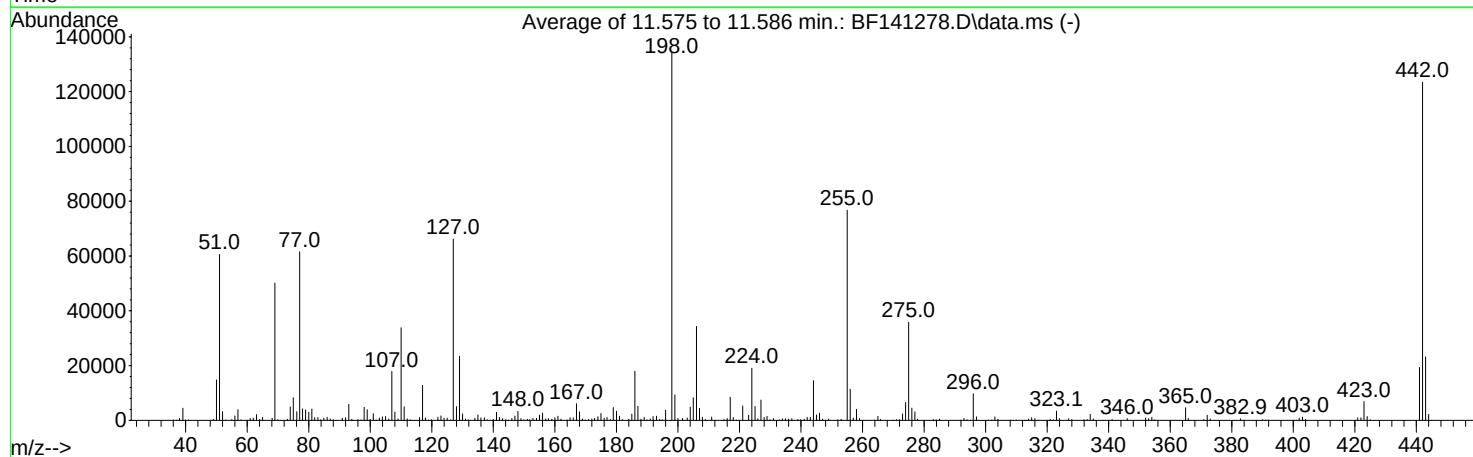


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012825\
Data File : BF141278.D
Acq On : 28 Jan 2025 14:05
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF012825.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Jan 28 23:51:29 2025

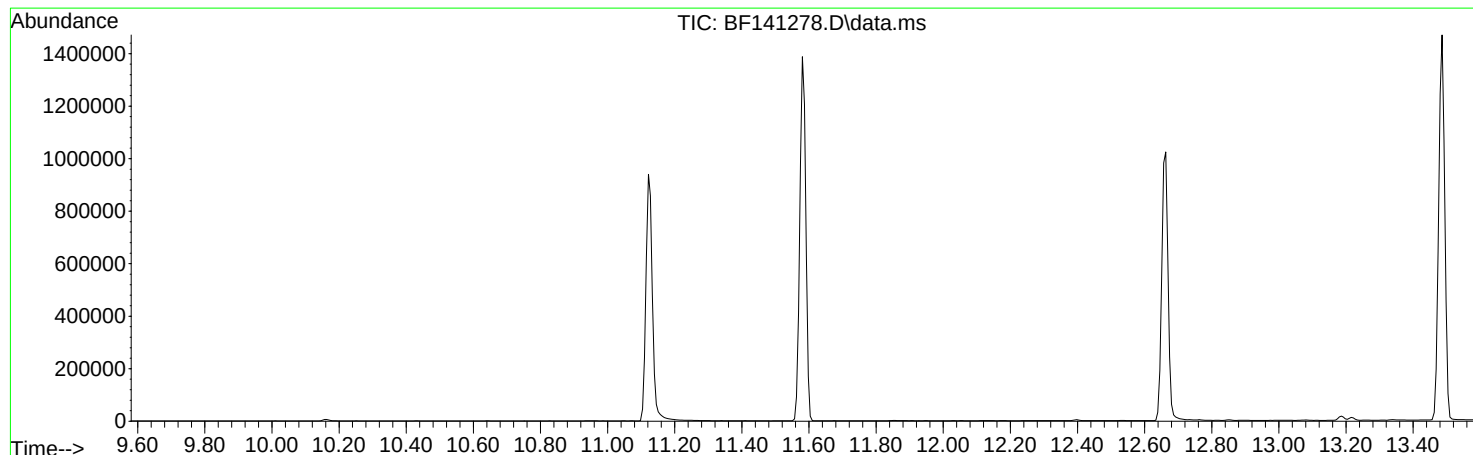




AutoFind: Scans 1612, 1613, 1614; Background Corrected with Scan 1606

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
51	198	10	80	45.1	60573	PASS
68	69	0.00	2	1.6	815	PASS
69	198	0.00	100	37.3	50101	PASS
70	69	0.00	2	0.5	232	PASS
127	198	10	80	49.3	66181	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	134285	PASS
199	198	5	9	6.9	9319	PASS
275	198	10	60	26.7	35795	PASS
365	198	1	100	3.4	4592	PASS
441	198	0.01	100	14.4	19359	PASS
442	442	50	100	100.0	123403	PASS
443	442	15	24	18.8	23167	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012825\
Data File : BF141278.D
Acq On : 28 Jan 2025 14:05
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jan 28 16:06:02 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF012825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 28 16:04:53 2025
Response via : Initial Calibration

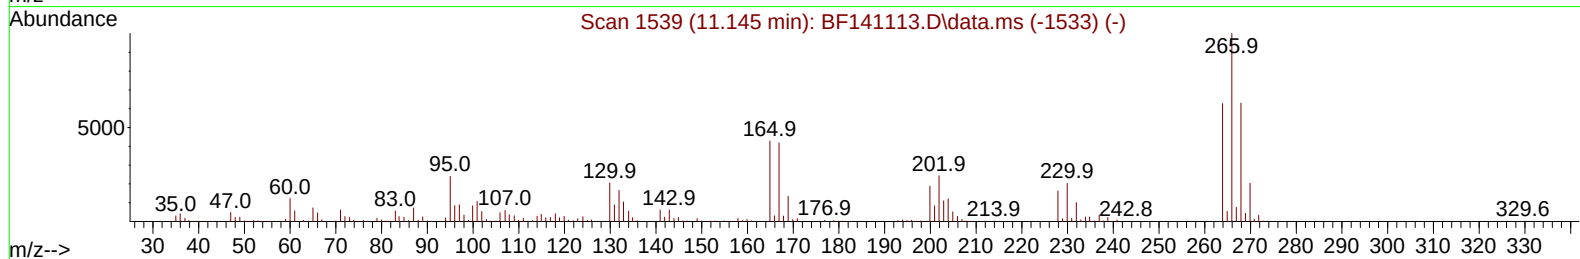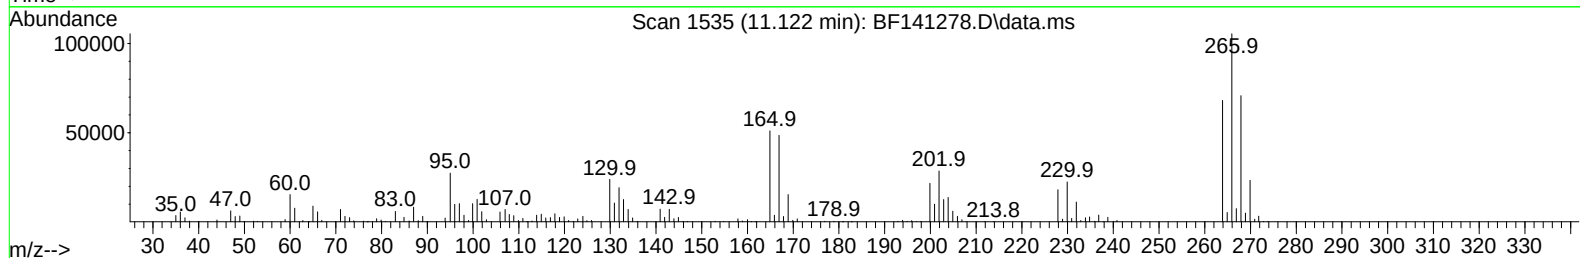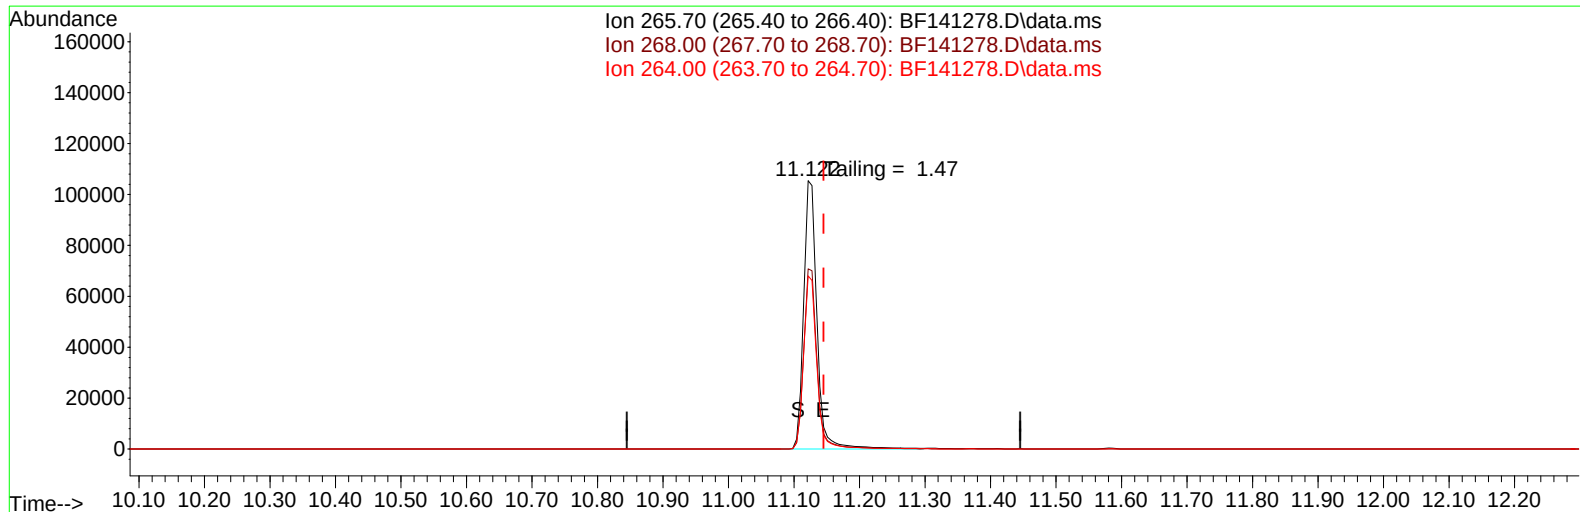

TIC: BF141278.D\data.ms

(70) Pentachlorophenol (C)

11.122min (-0.024) 27251.84 ng




response 149187

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.00	67.15
264.00	62.70	64.53
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012825\
Data File : BF141278.D
Acq On : 28 Jan 2025 14:05
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jan 28 16:06:02 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF012825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 28 16:04:53 2025
Response via : Initial Calibration

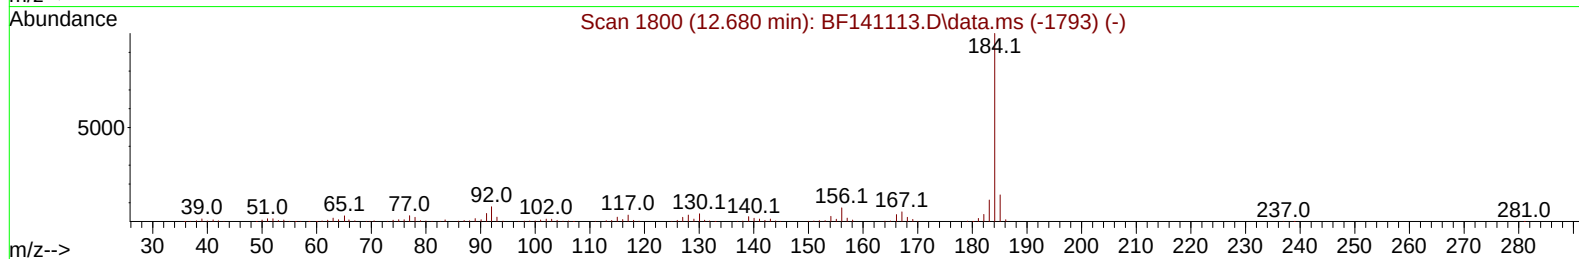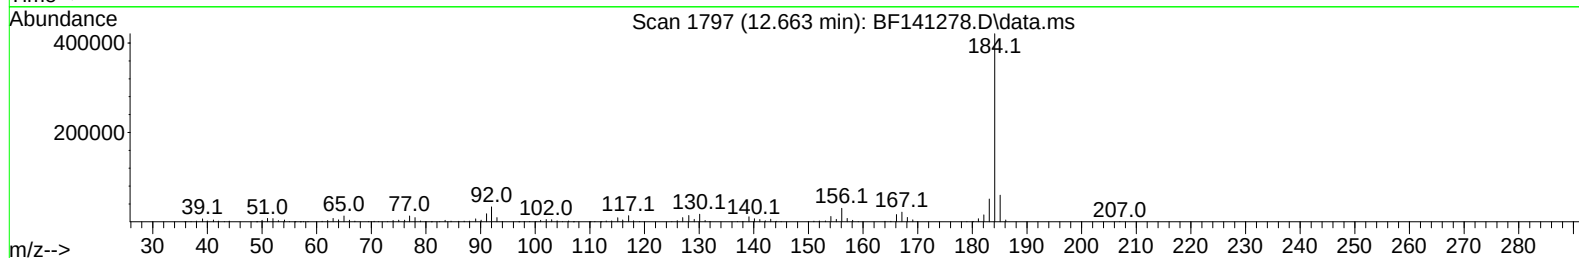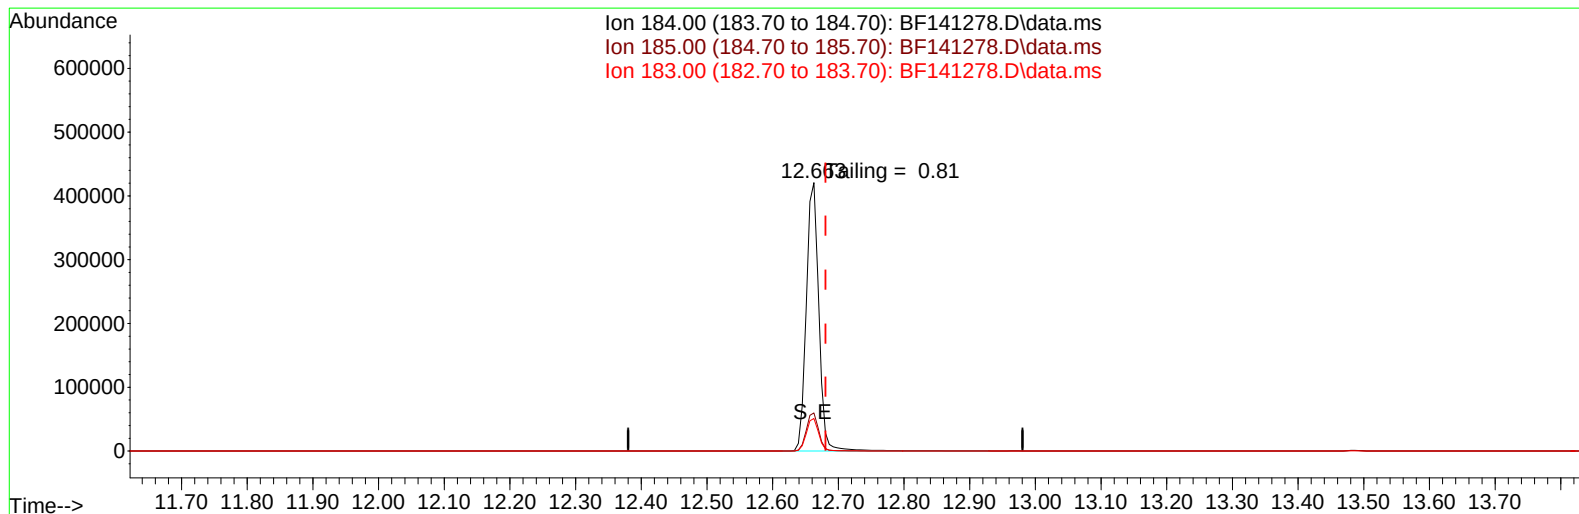

TIC: BF141278.D\data.ms

(77) Benzidine

12.663min (-0.018) 0.00 ng

response 556712

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	14.18
183.00	11.50	12.10
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
1/28/2025	BNA_F	<u>BF141278.D</u>
Compound Name	Response	Retention Time
DDT	360480	13.486
DDD	8572	13.186
DDE	643	12.851
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
9215	369695	2.49

Instrument :
BNA_F
ClientSampleId :
DFTPP