

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF012915\
 Data File : BF077128.D
 Acq On : 29 Jan 2015 17:37
 Operator : TP/IZ
 Sample : PB81560BL
 Misc : S
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB81560BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF011415.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	18	20	24	rBV	10345	19264	2.25%	0.290%
2	1.384	24	26	35	rVB	42182	79855	9.32%	1.201%
3	3.738	229	232	241	rBV	36437	93992	10.97%	1.414%
4	4.698	314	316	331	rVB	286690	646527	75.43%	9.724%
5	7.099	522	526	530	rBV	354055	599328	69.92%	9.014%
6	7.179	530	533	537	rVB	384803	684732	79.89%	10.299%
7	7.682	574	577	581	rBV	110203	171077	19.96%	2.573%
8	8.002	602	605	610	rBV	328000	509007	59.39%	7.656%
9	8.985	688	691	696	rBV	255346	393223	45.88%	5.914%
10	10.596	828	832	836	rBV	137978	241248	28.15%	3.628%
11	13.248	1060	1064	1067	rBV	501313	759538	88.62%	11.424%
12	14.711	1189	1192	1196	rBV	169940	264276	30.83%	3.975%
13	14.779	1196	1198	1206	rBV2	5214	11327	1.32%	0.170%
14	16.448	1341	1344	1347	rBV	316055	475889	55.52%	7.157%
15	17.568	1439	1442	1445	rBV	224883	274850	32.07%	4.134%
16	19.809	1636	1638	1641	rBV	767215	857109	100.00%	12.891%
17	21.066	1746	1748	1751	rVB	228650	286736	33.45%	4.313%
18	22.712	1889	1892	1895	rBV	242779	280866	32.77%	4.224%


Sum of corrected areas: 6648844

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF012915\
Data File : BF077128.D
Acq On : 29 Jan 2015 17:37
Operator : TP/IZ
Sample : PB81560BL
Misc : S
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB81560BL

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF011415.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

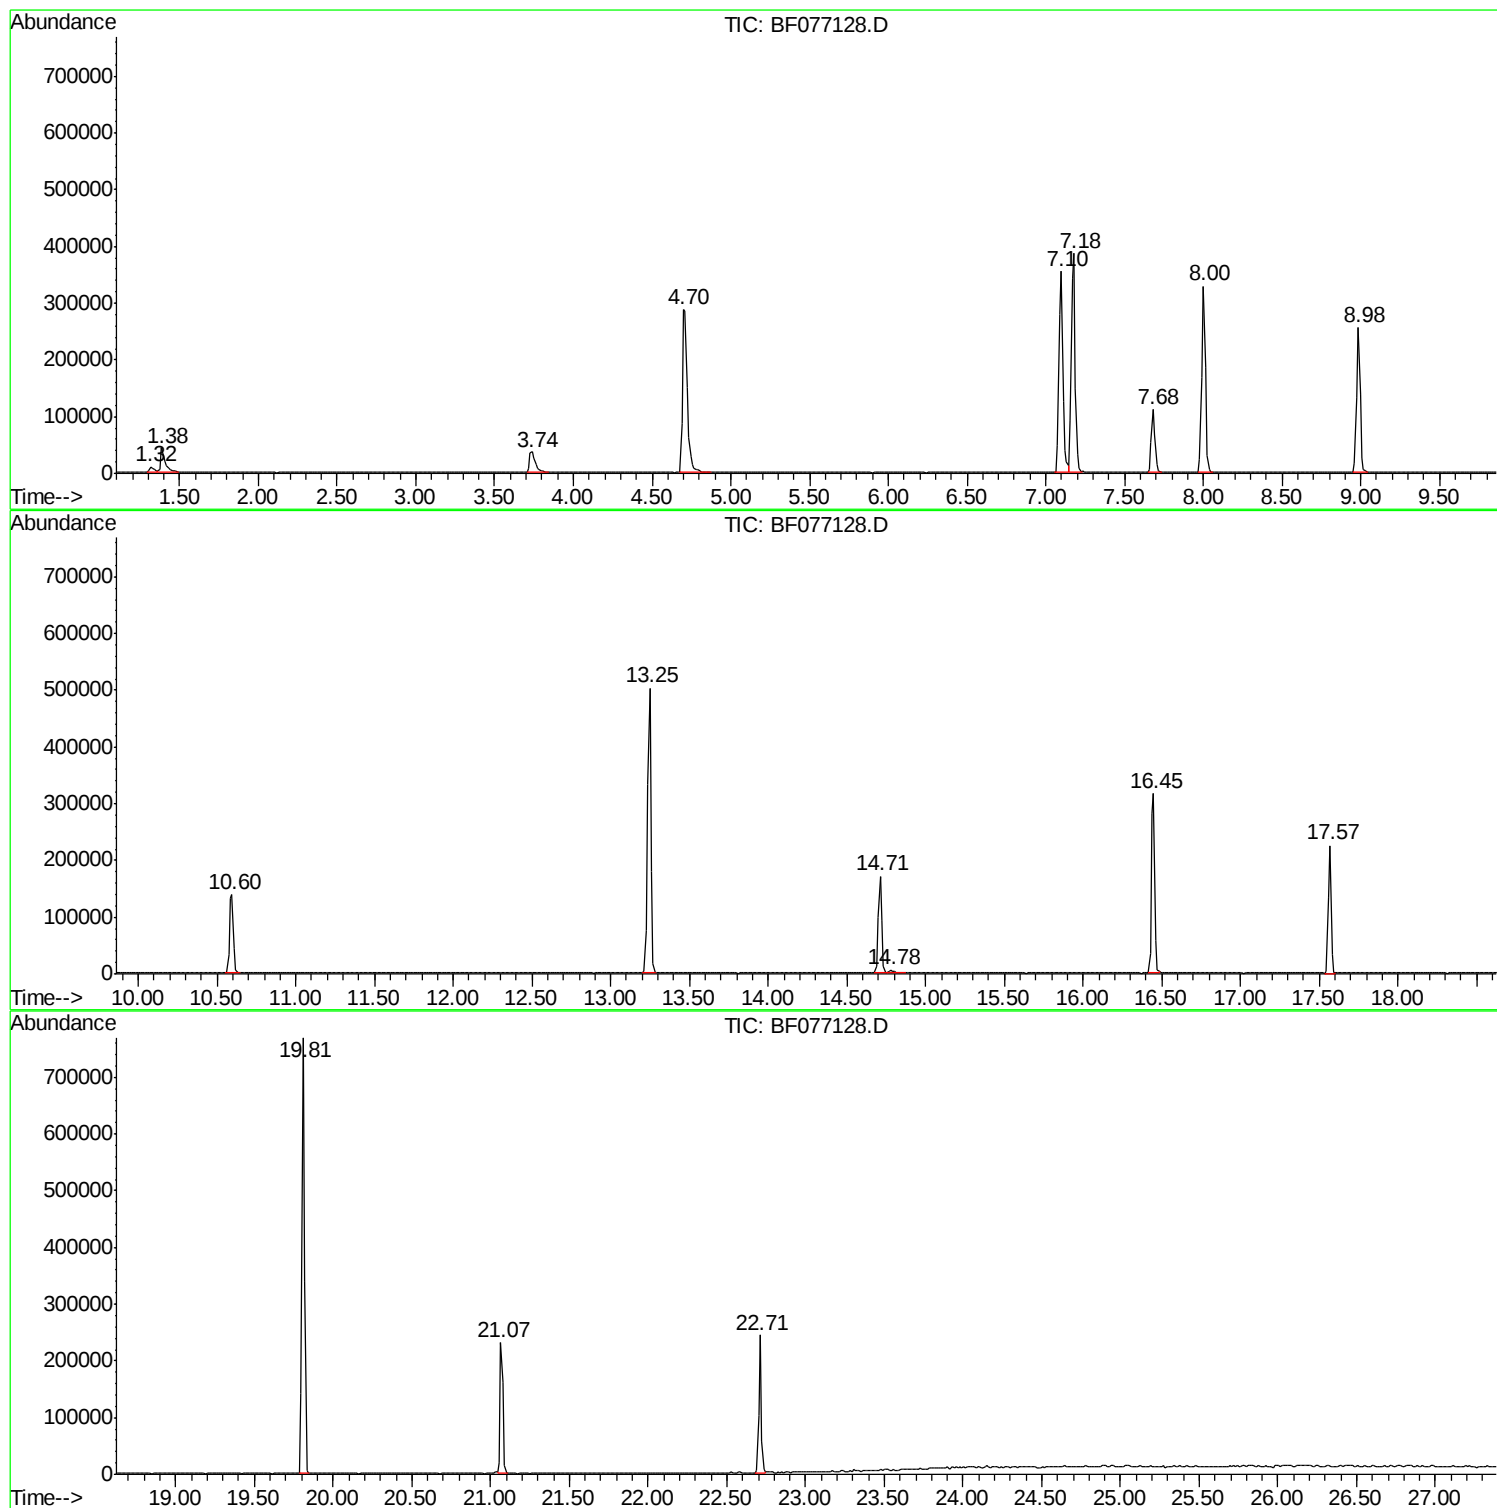

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF012915\
Data File : BF077128.D
Acq On : 29 Jan 2015 17:37
Operator : TP/IZ
Sample : PB81560BL
Misc : S
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB81560BL










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF011415.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 3 unknown3.74 Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.74	10.99 ng	93992	1,4-Dichlorobenzene-d4	7.68

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	40		
2	Guanidine	59	CH5N3	000113-00-8	9		
3	Silane, ethyldimethyl-	88	C4H12Si	000758-21-4	9		
4	2-Nonanone, 9-hydroxy-	158	C9H18O2	025368-56-3	9		
5	1-Propen-2-ol, acetate	100	C5H8O2	000108-22-5	9		

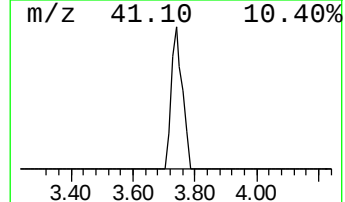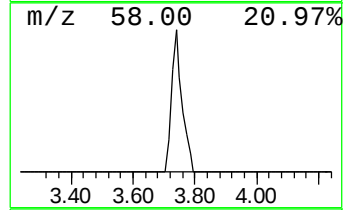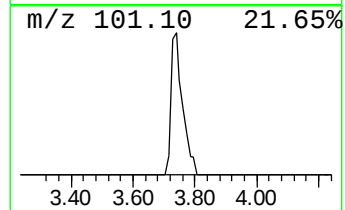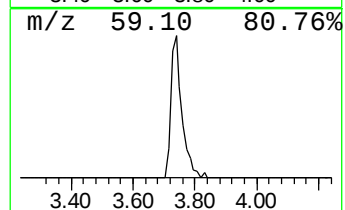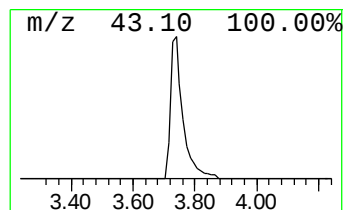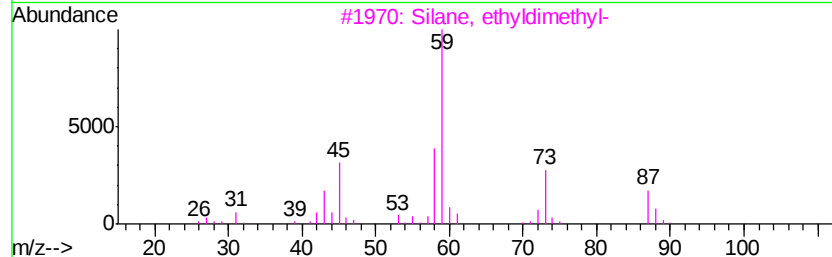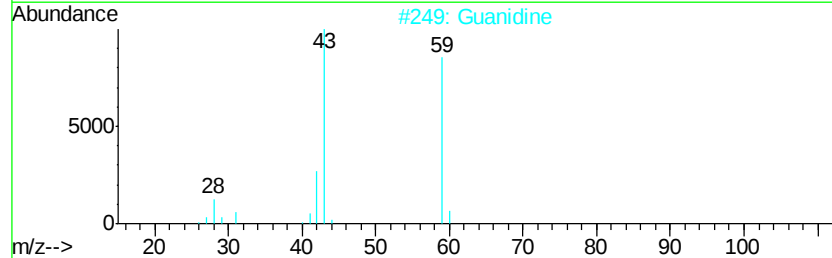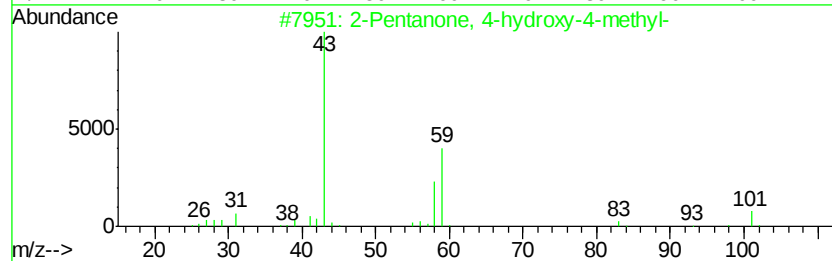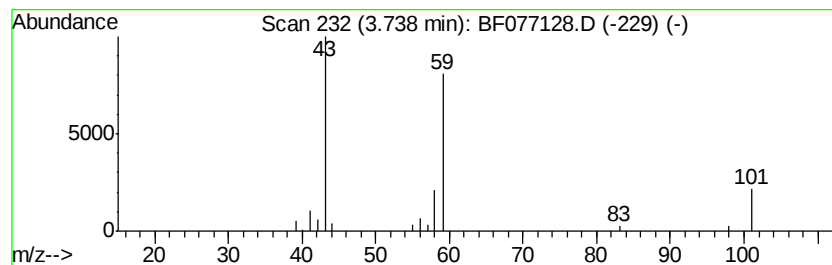

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF012915\
Data File : BF077128.D
Acq On : 29 Jan 2015 17:37
Operator : TP/IZ
Sample : PB81560BL
Misc : S
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB81560BL










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF011415.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 4 unknown7.18 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.18	80.05 ng	684732	1,4-Dichlorobenzene-d4	7.68

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	17
2		5-Aminoindole	132	C8H8N2	005192-03-0	12
3		Bicyclo[4.2.0]octa-1,3,5-triene,...	132	C10H12	028749-81-7	9
4		1,3,4-Thiadiazole-2(3H)-thione, ...	132	C3H4N2S2	029490-19-5	9
5		4-Chloro-2-fluoro-pyrimidine	132	C4H2ClFN2	051422-00-5	9

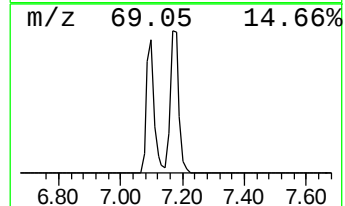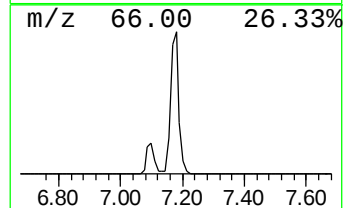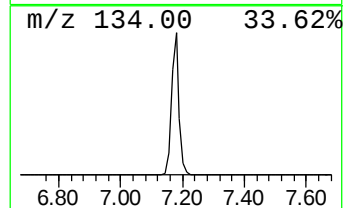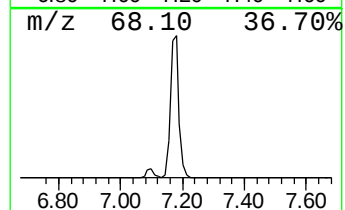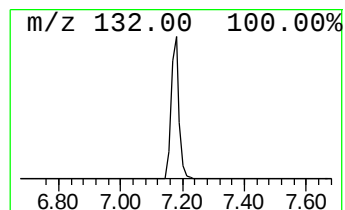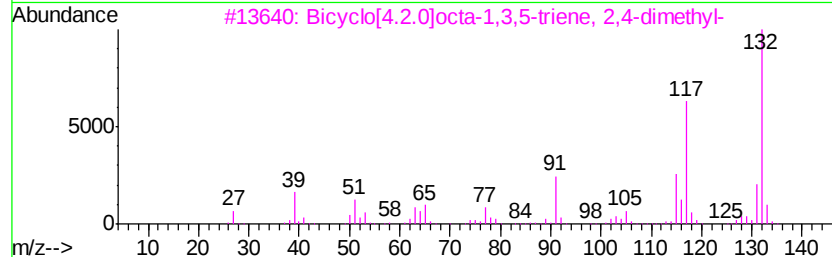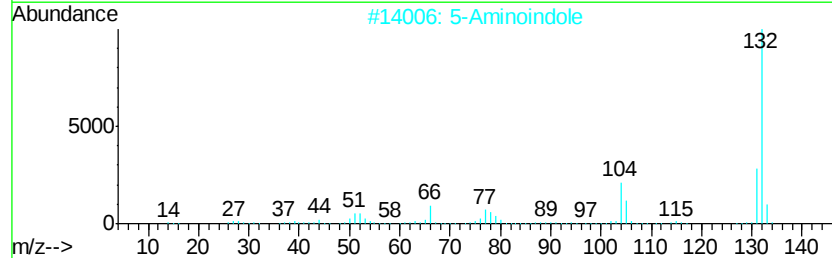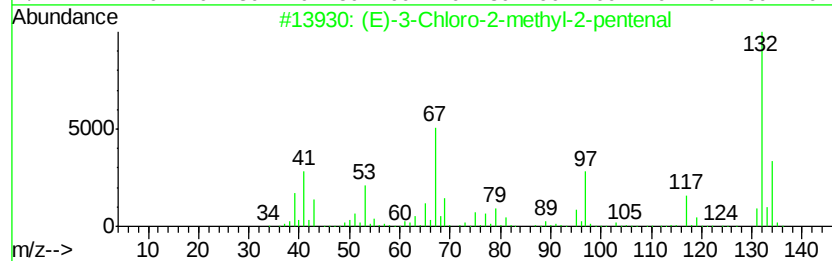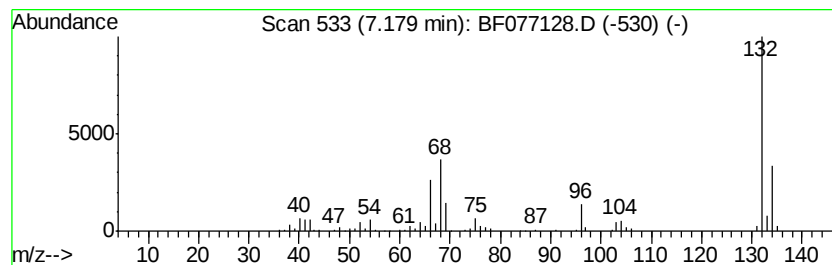

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF012915\
Data File : BF077128.D
Acq On : 29 Jan 2015 17:37
Operator : TP/IZ
Sample : PB81560BL
Misc : S
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB81560BL

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF011415.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown3.74	3.74	11.0	ng	93992	1	7.68	171077	20.0
unknown7.18	7.18	80.0	ng	684732	1	7.68	171077	20.0