


Data Path : Z:\HPCHEM1\BNA_F\Data\BF012915\
 Data File : BF077122.D
 Acq On : 29 Jan 2015 13:34
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF011415.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jan 28 16:07:35 2015

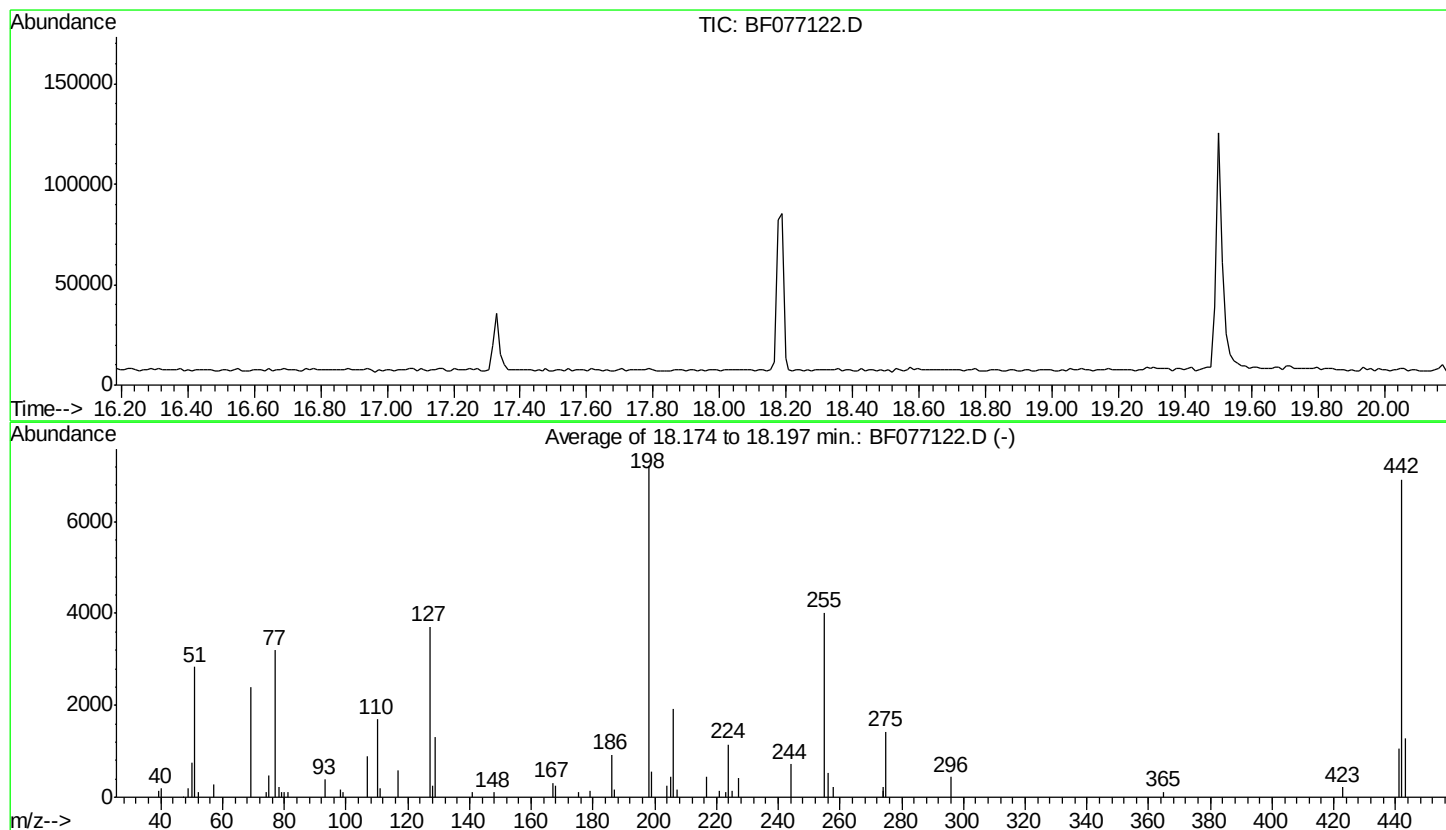

AutoFind: Scans 1495, 1496, 1497; Background Corrected with Scan 1491

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.3	2838	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	33.4	2408	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	51.4	3708	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	7218	PASS
199	198	5	9	7.6	552	PASS
275	198	10	60	19.8	1431	PASS
365	198	1	100	1.6	115	PASS
441	442	0.01	24	15.1	1048	PASS
442	198	50	100	95.9	6919	PASS
443	442	15	24	18.4	1270	PASS