


Data Path : Z:\HPCHEM1\BNA_F\Data\BF012915\
 Data File : BF077138.D
 Acq On : 30 Jan 2015 1:04
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF011415.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jan 28 16:07:35 2015

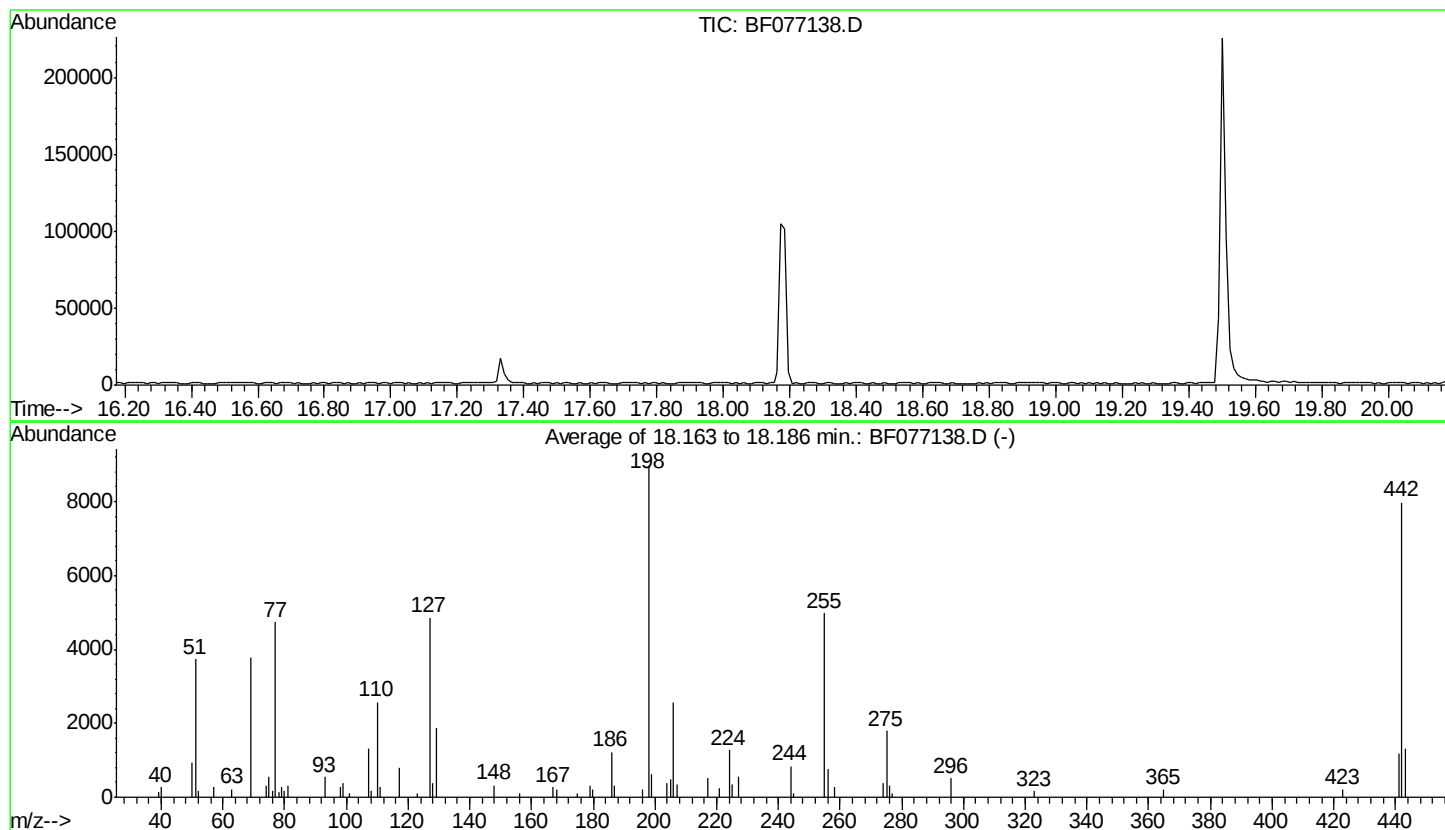

AutoFind: Scans 1494, 1495, 1496; Background Corrected with Scan 1491

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.6	3735	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	42.0	3769	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	54.1	4850	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	8970	PASS
199	198	5	9	7.0	627	PASS
275	198	10	60	20.1	1800	PASS
365	198	1	100	2.3	206	PASS
441	442	0.01	24	14.8	1182	PASS
442	198	50	100	88.8	7966	PASS
443	442	15	24	16.7	1329	PASS