
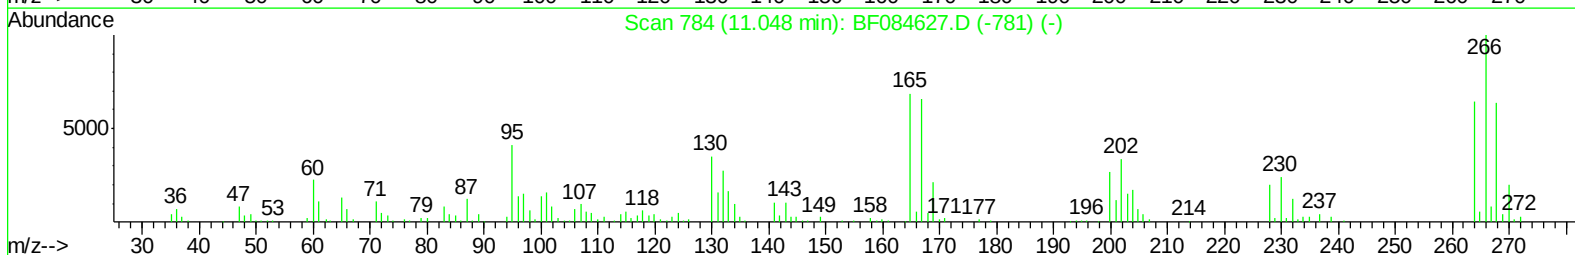
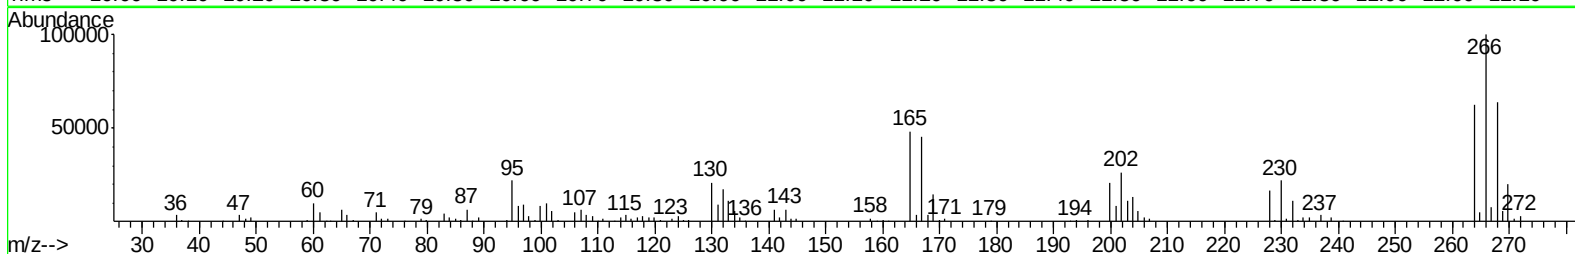


Data Path : Z:\HPCHEM1\BNA_F\Data\BF012916\
Data File : BF084645.D
Acq On : 29 Jan 2016 19:28
Operator : SJ/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 01 02:49:53 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF012916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 29 12:54:53 2016
Response via : Initial Calibration

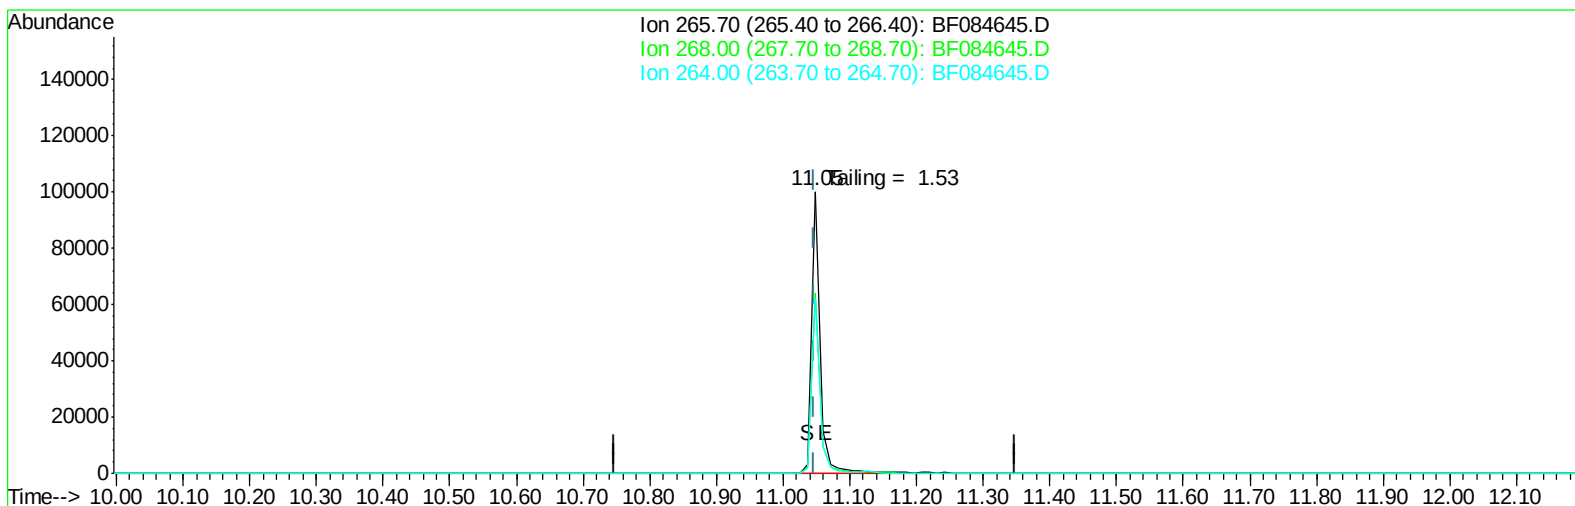

TIC: BF084645.D

(69) Pentachlorophenol (C)




11.048min (-0.000) 0.00ng

response 88767

Ion	Exp%	Act%
265.70	100	100
268.00	65.50	63.92
264.00	62.70	62.21
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\Data\BF012916\
Data File : BF084645.D
Acq On : 29 Jan 2016 19:28
Operator : SJ/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 01 02:49:53 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF012916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 29 12:54:53 2016
Response via : Initial Calibration

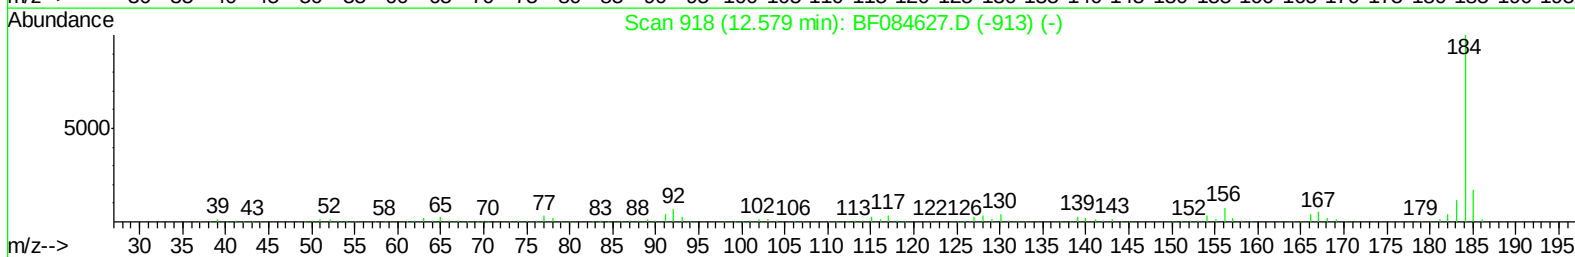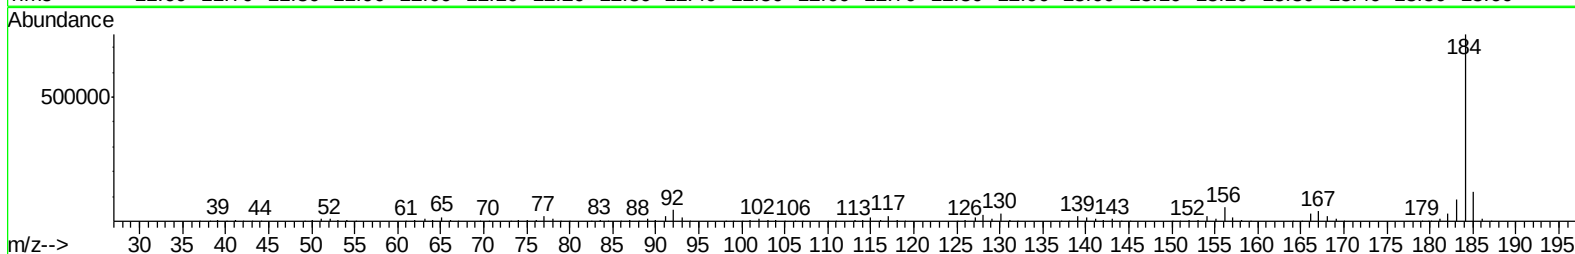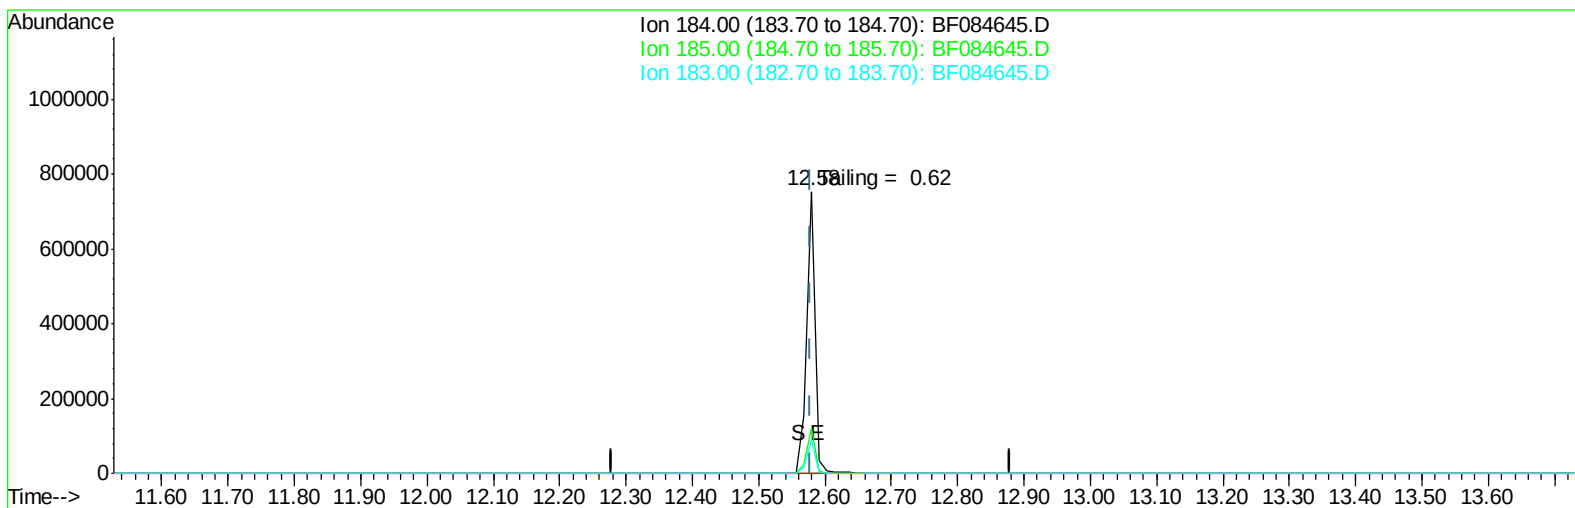

TIC: BF084645.D

(76) Benzidine

12.579min (-0.000) 0.00ng

response 660488

Ion	Exp%	Act%
184.00	100	100
185.00	15.20	15.77
183.00	12.30	11.77
0.00	0.00	0.00