


Data Path : Z:\HPCHEM1\BNA F\Data\BF012916\  
 Data File : BF084623.D  
 Acq On : 29 Jan 2016 8:44  
 Operator : SJ/IZ  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA\_F\METHODS\8270-BF012916.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Fri Jan 29 12:54:53 2016

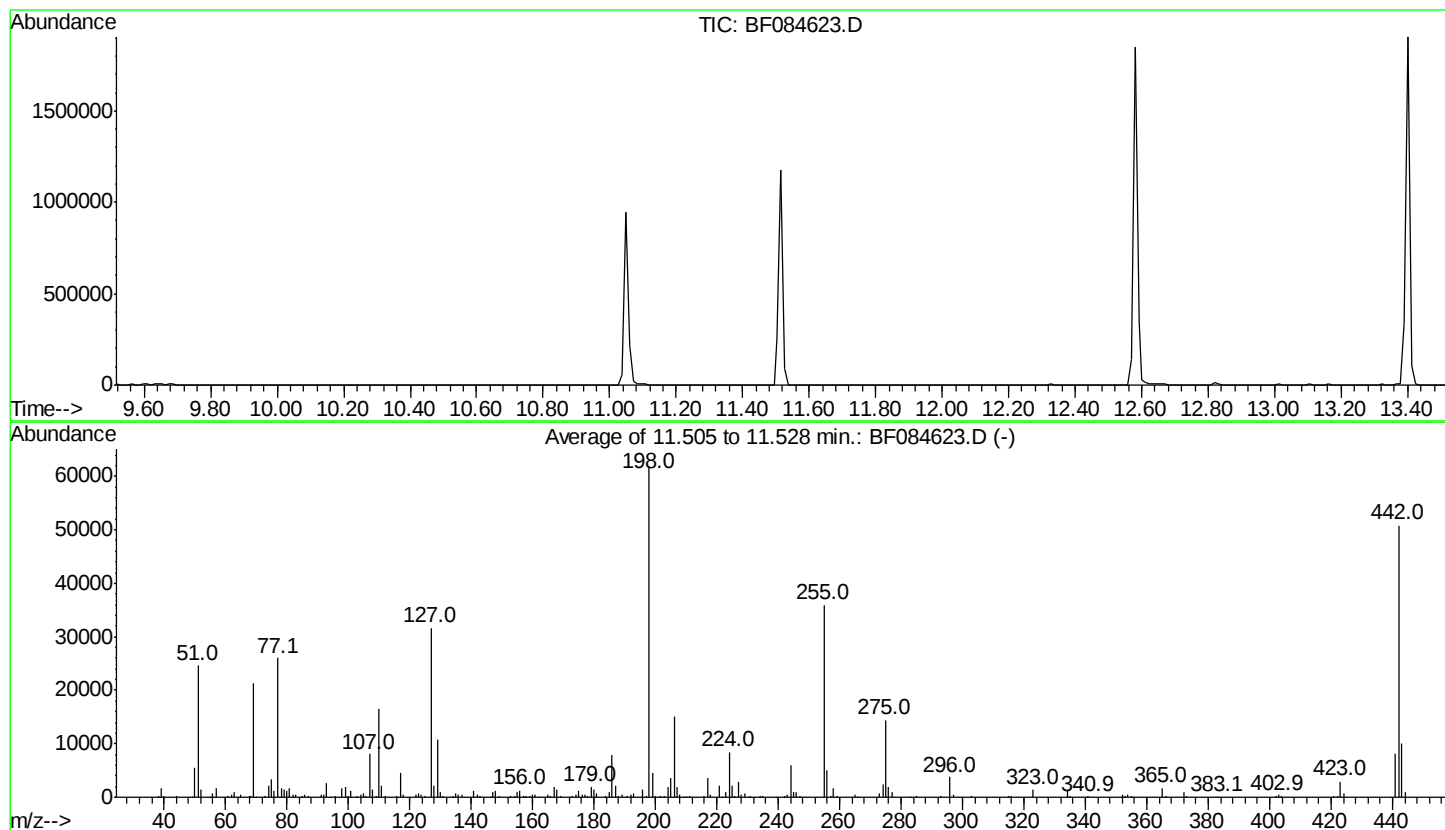

AutoFind: Scans 824, 825, 826; Background Corrected with Scan 820

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 39.7      | 24640   | PASS             |
| 68          | 69           | 0.00         | 2            | 1.1       | 227     | PASS             |
| 69          | 198          | 0.00         | 100          | 34.2      | 21217   | PASS             |
| 70          | 69           | 0.00         | 2            | 0.5       | 101     | PASS             |
| 127         | 198          | 10           | 80           | 51.1      | 31680   | PASS             |
| 197         | 198          | 0.00         | 2            | 0.6       | 347     | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 62005   | PASS             |
| 199         | 198          | 5            | 9            | 7.2       | 4494    | PASS             |
| 275         | 198          | 10           | 60           | 23.3      | 14478   | PASS             |
| 365         | 198          | 1            | 100          | 2.8       | 1731    | PASS             |
| 441         | 442          | 0.01         | 24           | 16.1      | 8155    | PASS             |
| 442         | 198          | 50           | 100          | 81.8      | 50749   | PASS             |
| 443         | 442          | 15           | 24           | 19.8      | 10031   | PASS             |