


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF012916\
 Data File : BF084645.D
 Acq On : 29 Jan 2016 19:28
 Operator : SJ/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF012916.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jan 29 12:54:53 2016

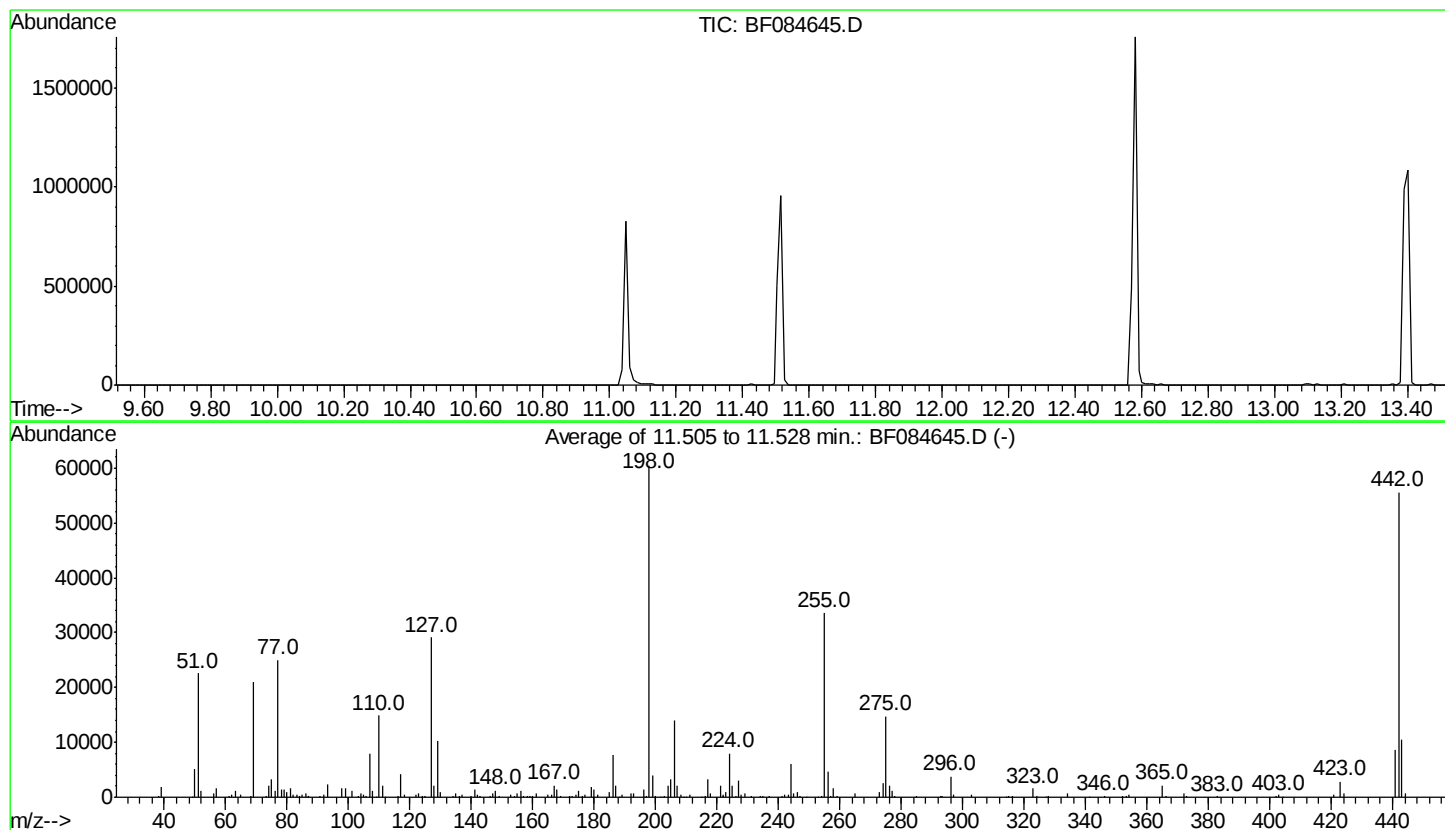

AutoFind: Scans 824, 825, 826; Background Corrected with Scan 820

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.3	22566	PASS
68	69	0.00	2	1.6	339	PASS
69	198	0.00	100	34.9	21064	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	48.2	29120	PASS
197	198	0.00	2	0.6	337	PASS
198	198	100	100	100.0	60439	PASS
199	198	5	9	6.4	3866	PASS
275	198	10	60	24.4	14726	PASS
365	198	1	100	3.6	2175	PASS
441	442	0.01	24	15.7	8703	PASS
442	198	50	100	91.9	55565	PASS
443	442	15	24	19.1	10587	PASS