
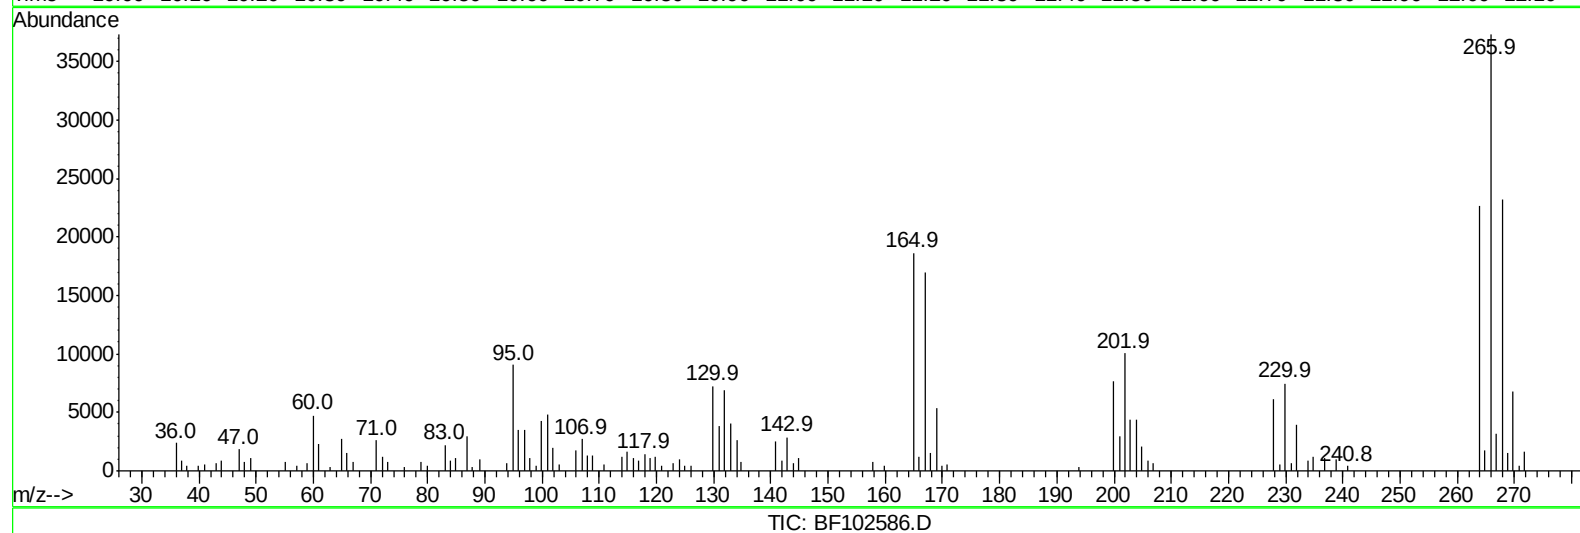


Data Path : U:\HPCHEM1\BNA F\DATA\BF012918\  
Data File : BF102586.D  
Acq On : 29 Jan 2018 8:53  
Operator : SJ/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 30 06:28:27 2018  
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF012218.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Sat Jan 27 20:48:40 2018  
Response via : Initial Calibration

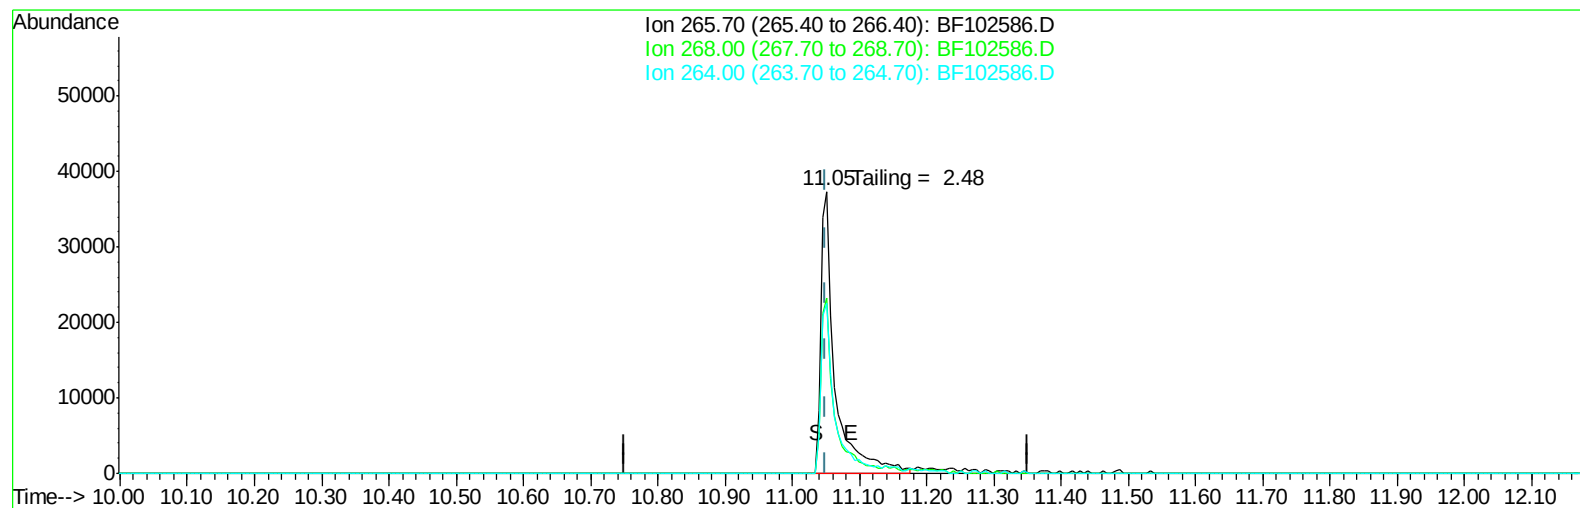

(69) Pentachlorophenol (C)



11.051min (+0.000) 27918.22ng

response 55619

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 265.70 | 100   | 100   |
| 268.00 | 63.90 | 62.19 |
| 264.00 | 61.90 | 60.67 |
| 0.00   | 0.00  | 0.00  |

Data Path : U:\HPCHEM1\BNA F\DATA\BF012918\  
Data File : BF102586.D  
Acq On : 29 Jan 2018 8:53  
Operator : SJ/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 30 06:28:27 2018  
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF012218.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Sat Jan 27 20:48:40 2018  
Response via : Initial Calibration

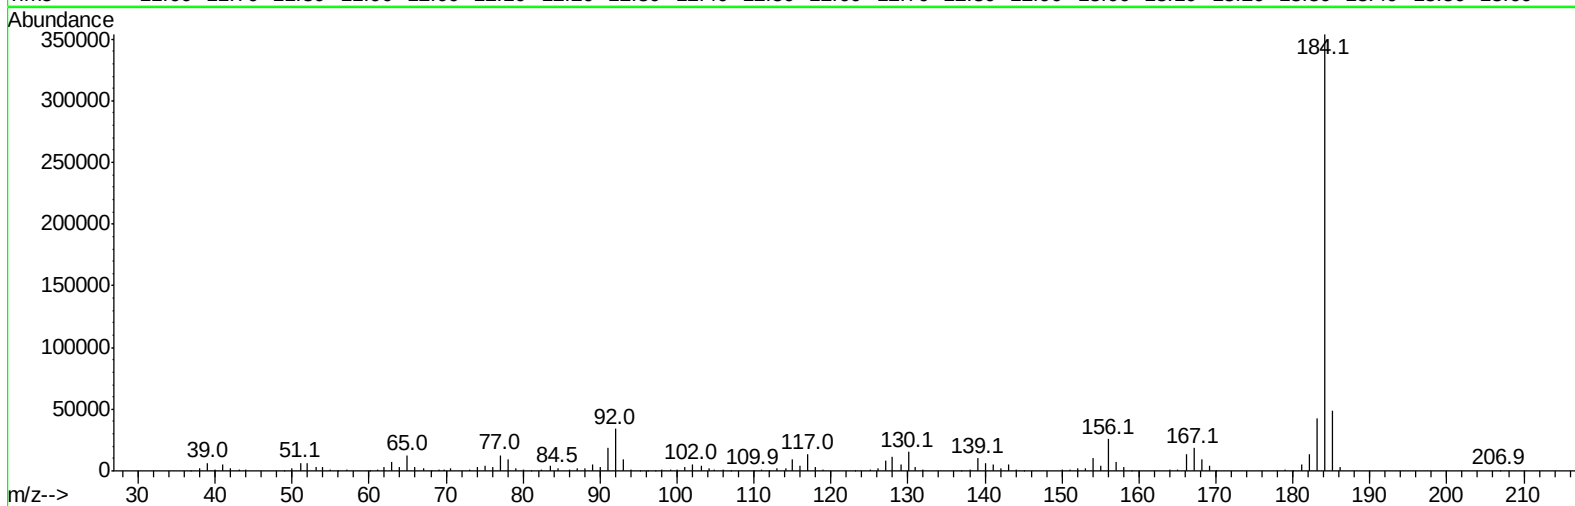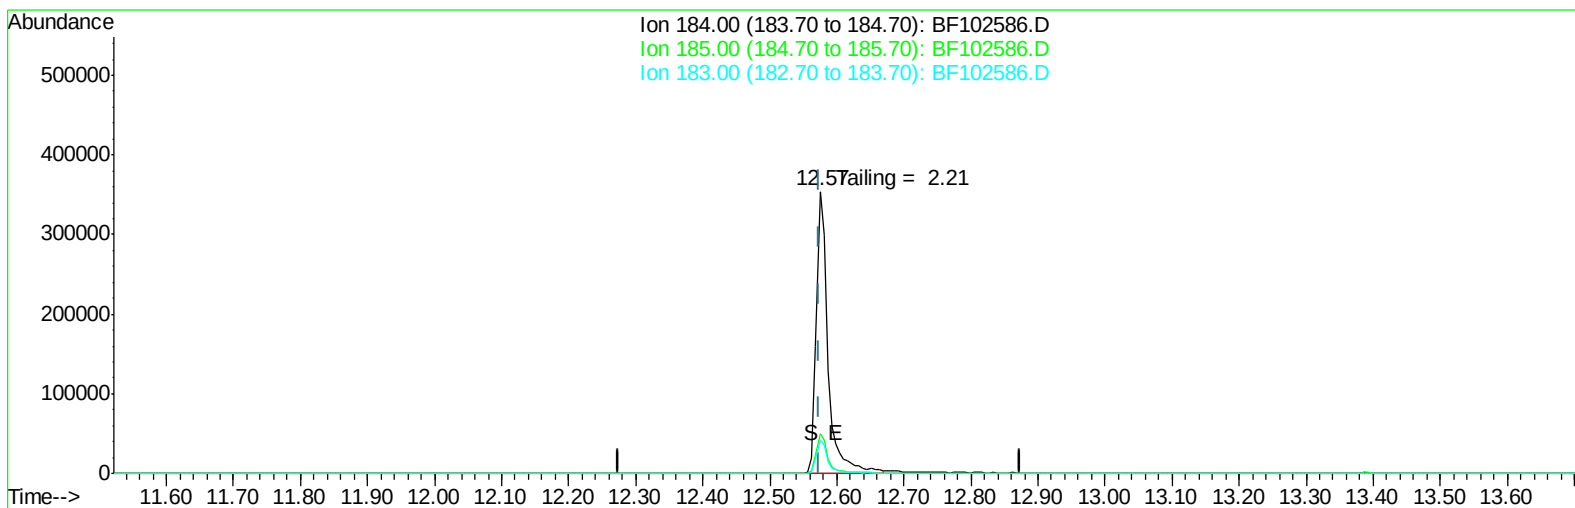

TIC: BF102586.D

(76) Benzidine

12.574min (+0.000) 0.00ng

response 423031

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 184.00 | 100   | 100   |
| 185.00 | 15.70 | 13.89 |
| 183.00 | 11.60 | 12.06 |
| 0.00   | 0.00  | 0.00  |