
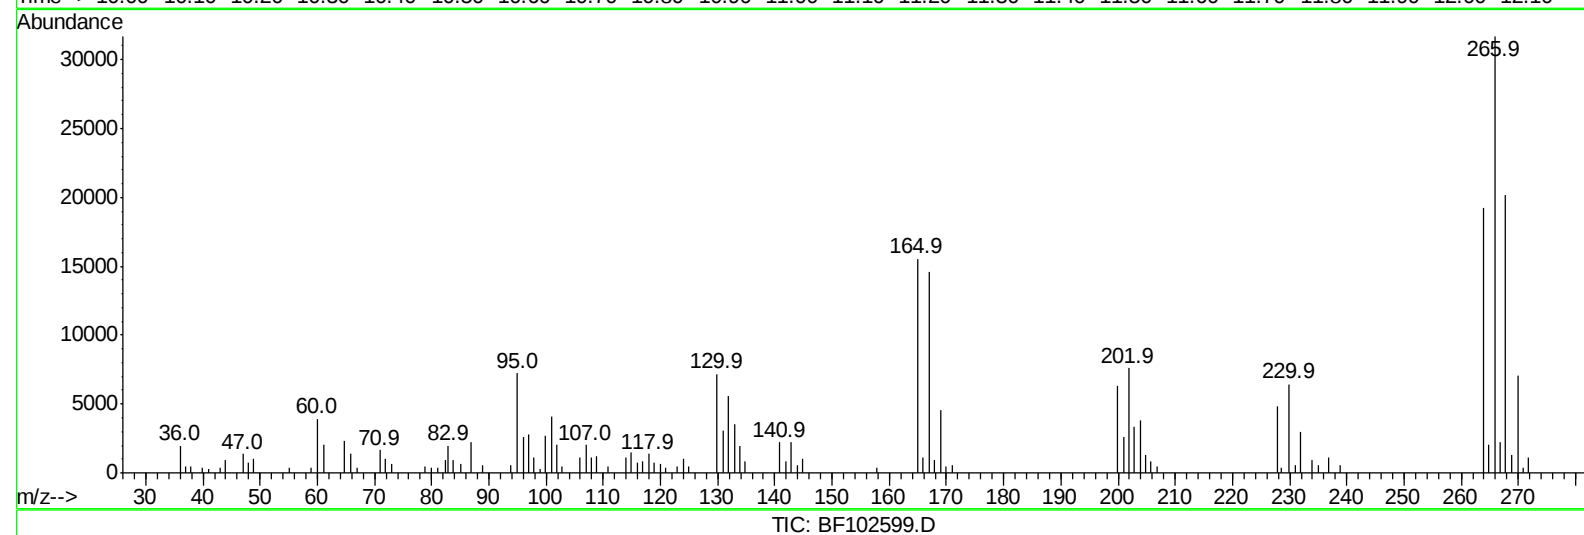


Data Path : U:\HPCHEM1\BNA F\DATA\BF012918\
Data File : BF102599.D
Acq On : 29 Jan 2018 16:14
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 30 00:07:59 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF012218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jan 27 20:48:40 2018
Response via : Initial Calibration

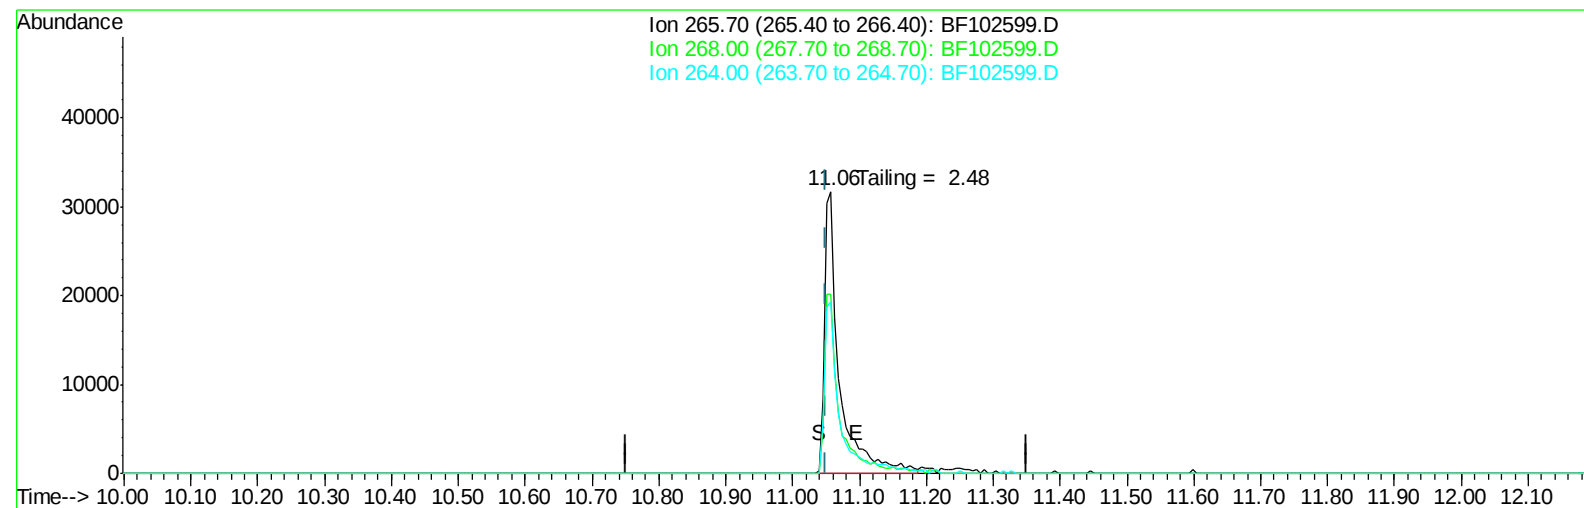

(69) Pentachlorophenol (C)



11.057min (+0.006) 22796.62ng

response 49741

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	63.57
264.00	61.90	60.82
0.00	0.00	0.00

Data Path : U:\HPCHEM1\BNA F\DATA\BF012918\
Data File : BF102599.D
Acq On : 29 Jan 2018 16:14
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 30 00:07:59 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF012218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jan 27 20:48:40 2018
Response via : Initial Calibration

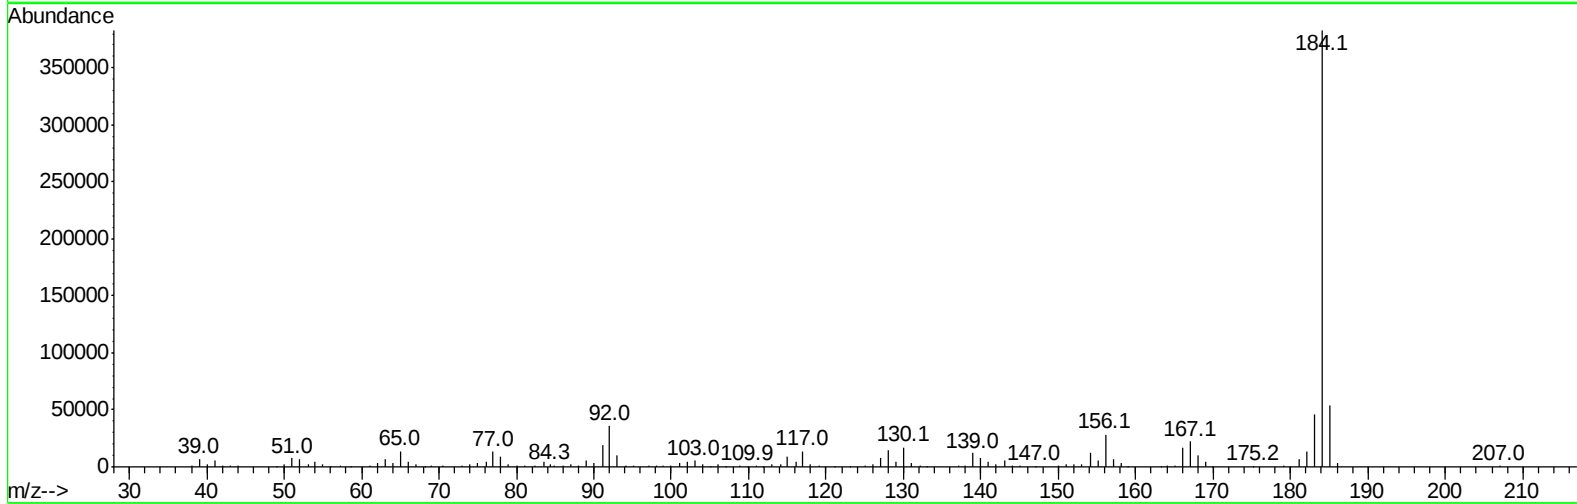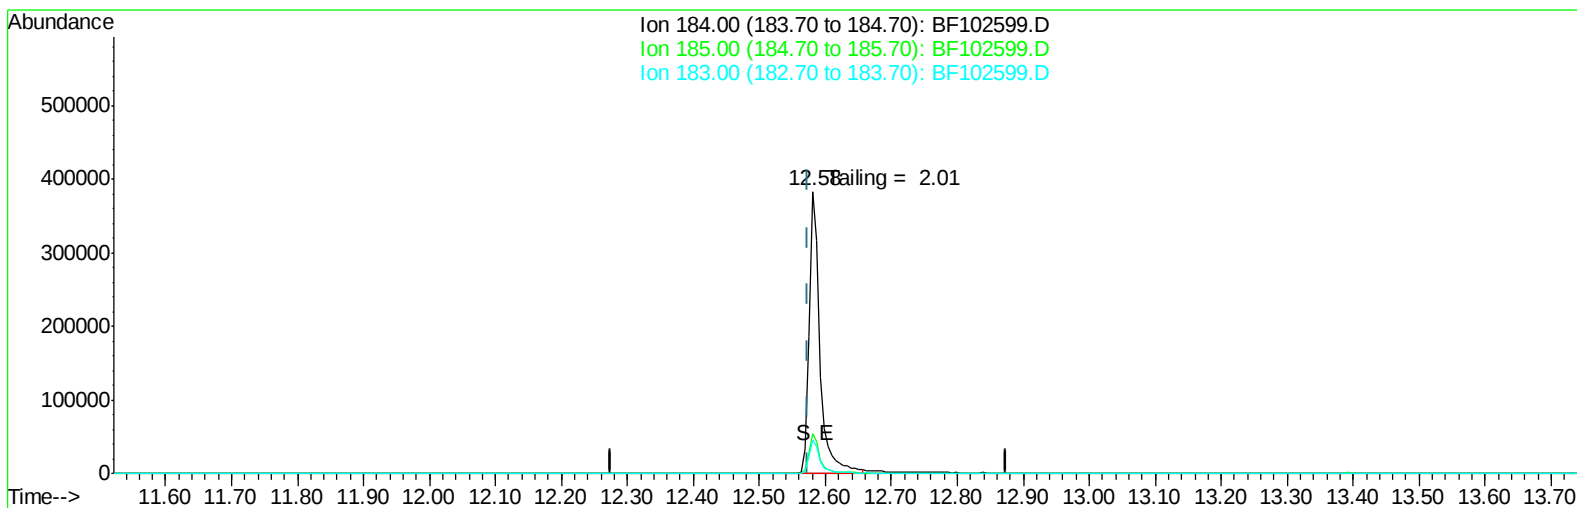

TIC: BF102599.D

(76) Benzidine

12.580min (+0.006) 122543.66ng

response 452835

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.21
183.00	11.60	12.00
0.00	0.00	0.00