


Data Path : Z:\HPCHEM1\BNA_F\Data\BF012918\
 Data File : BF102599.D
 Acq On : 29 Jan 2018 16:14
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF012218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Jan 27 20:48:40 2018

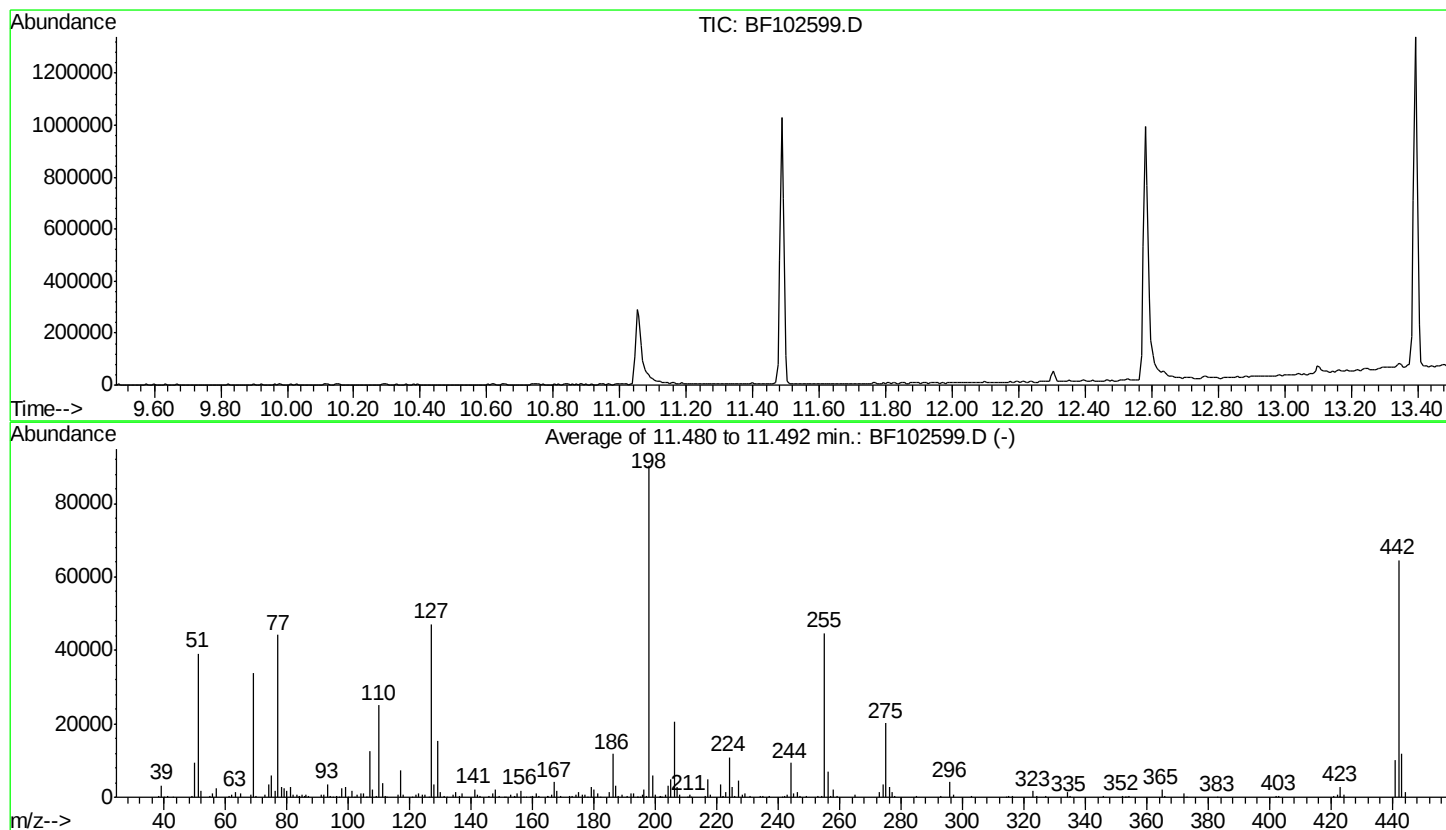

AutoFind: Scans 1597, 1598, 1599; Background Corrected with Scan 1592

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.4	39176	PASS
68	69	0.00	2	2.0	685	PASS
69	198	0.00	100	37.5	33841	PASS
70	69	0.00	2	0.7	230	PASS
127	198	10	80	52.2	47168	PASS
197	198	0.00	2	0.4	324	PASS
198	198	100	100	100.0	90293	PASS
199	198	5	9	6.5	5834	PASS
275	198	10	60	22.3	20174	PASS
365	198	1	100	2.2	1991	PASS
441	443	0.01	100	85.4	10149	PASS
442	198	50	100	71.5	64589	PASS
443	442	15	24	18.4	11888	PASS