


Data Path : Z:\HPCHEM1\BNA_F\Data\BF012918\
 Data File : BF102626.D
 Acq On : 30 Jan 2018 5:36
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF012218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Jan 27 20:48:40 2018

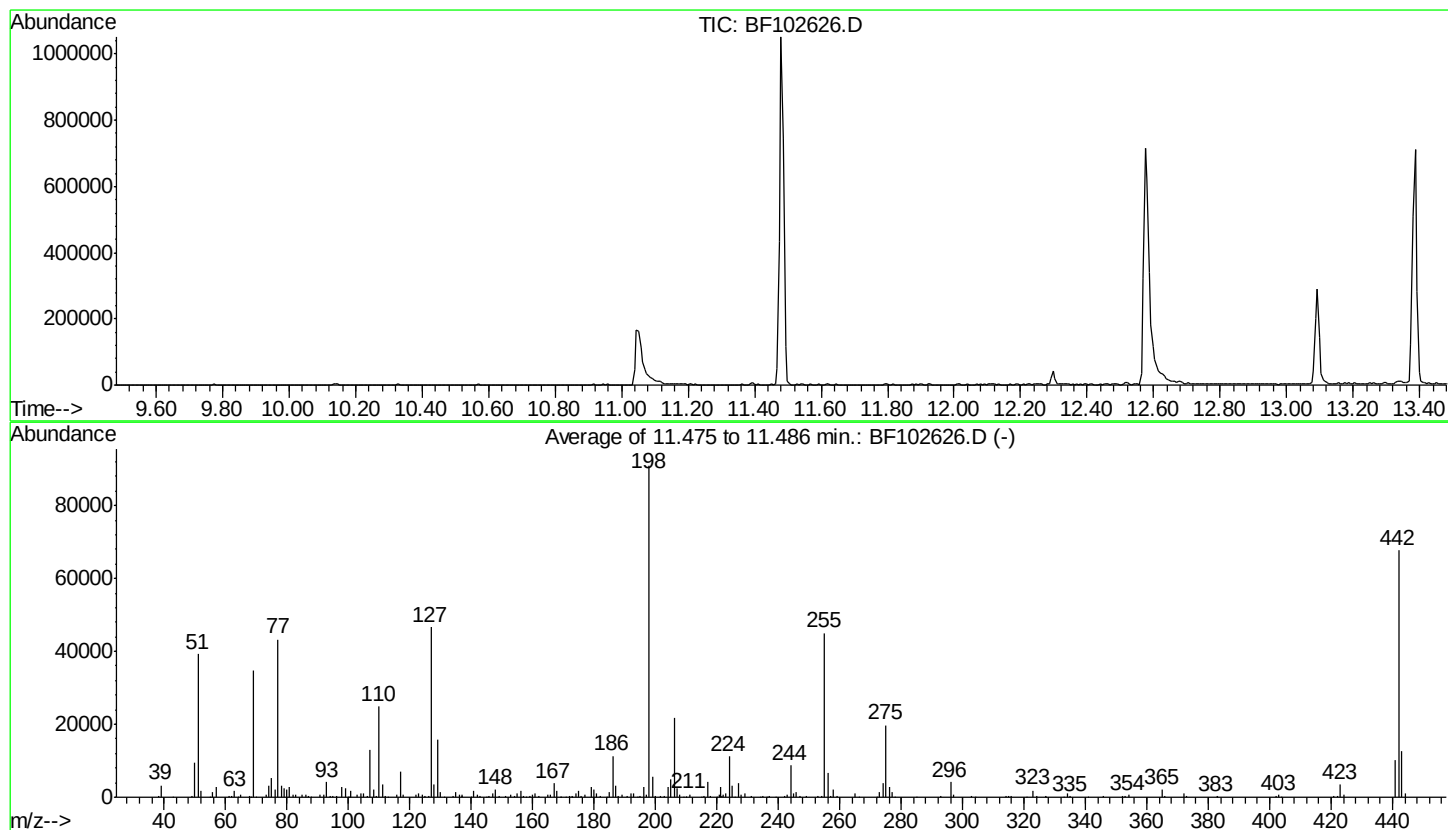

AutoFind: Scans 1596, 1597, 1598; Background Corrected with Scan 1592

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.2	39320	PASS
68	69	0.00	2	1.3	440	PASS
69	198	0.00	100	38.4	34920	PASS
70	69	0.00	2	0.3	104	PASS
127	198	10	80	51.3	46621	PASS
197	198	0.00	2	0.6	564	PASS
198	198	100	100	100.0	90946	PASS
199	198	5	9	6.3	5750	PASS
275	198	10	60	21.7	19742	PASS
365	198	1	100	2.1	1944	PASS
441	443	0.01	100	81.6	10263	PASS
442	198	50	100	74.4	67685	PASS
443	442	15	24	18.6	12577	PASS