
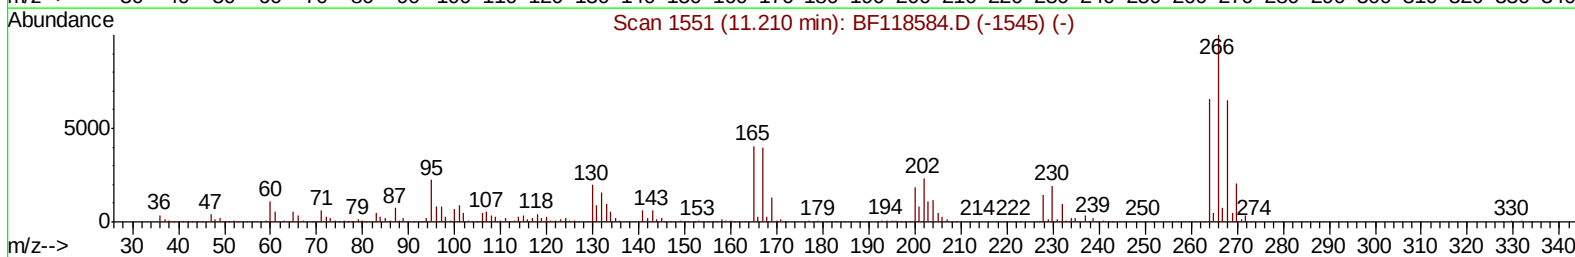
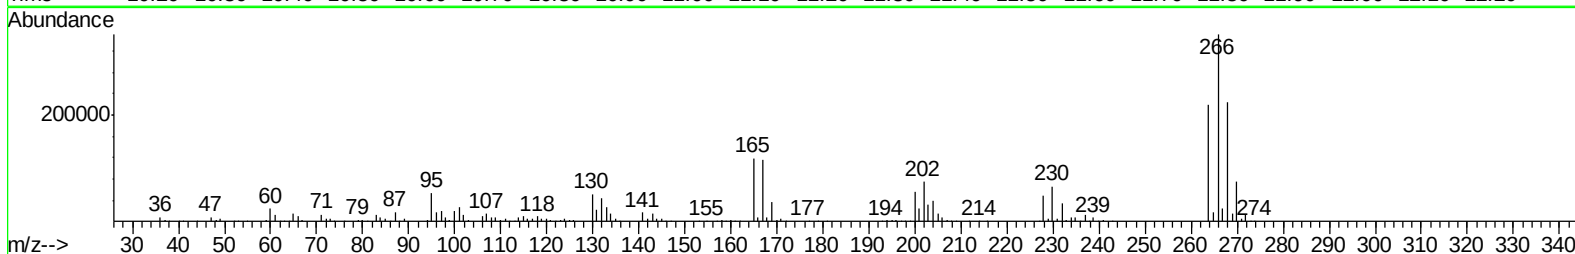


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF012920\
Data File : BF118725.D
Acq On : 29 Jan 2020 11:41
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 30 04:45:20 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF012020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 27 14:24:10 2020
Response via : Initial Calibration

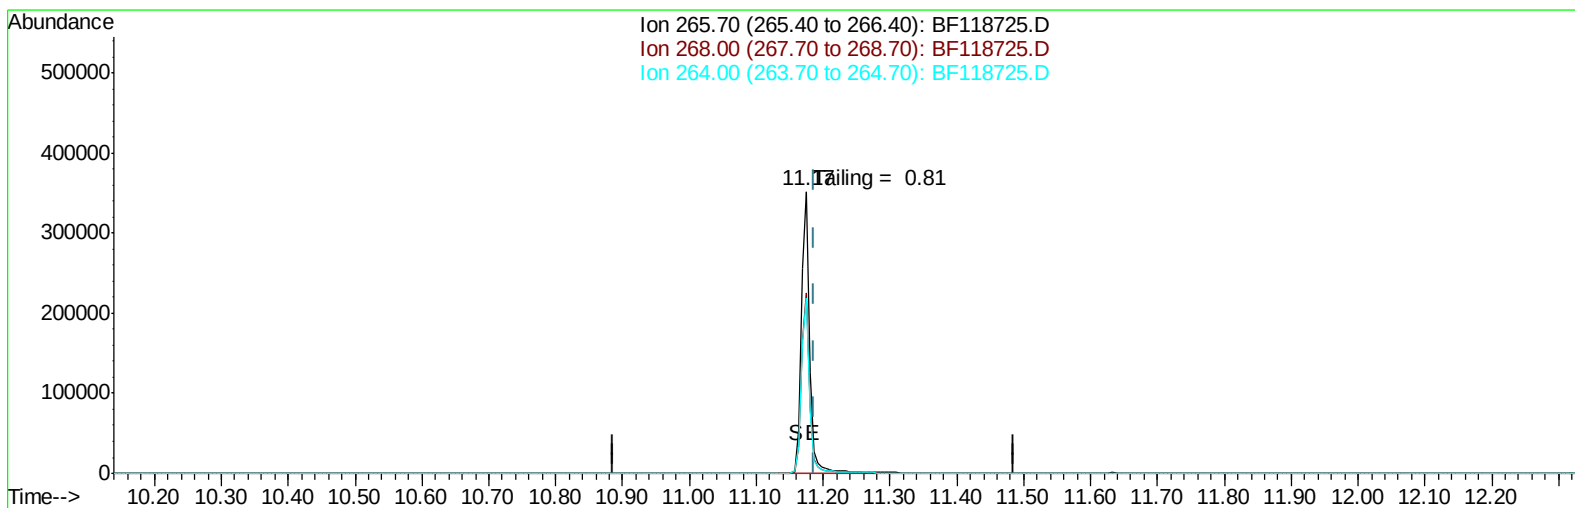

TIC: BF118725.D

(70) Pentachlorophenol (C)




11.174min (-0.012) 37028.58ng

response 312876

Ion	Exp%	Act%
265.70	100	100
268.00	64.50	63.95
264.00	63.60	62.24
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF012920\
 Data File : BF118725.D
 Acq On : 29 Jan 2020 11:41
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 30 04:45:20 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF012020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jan 27 14:24:10 2020
 Response via : Initial Calibration

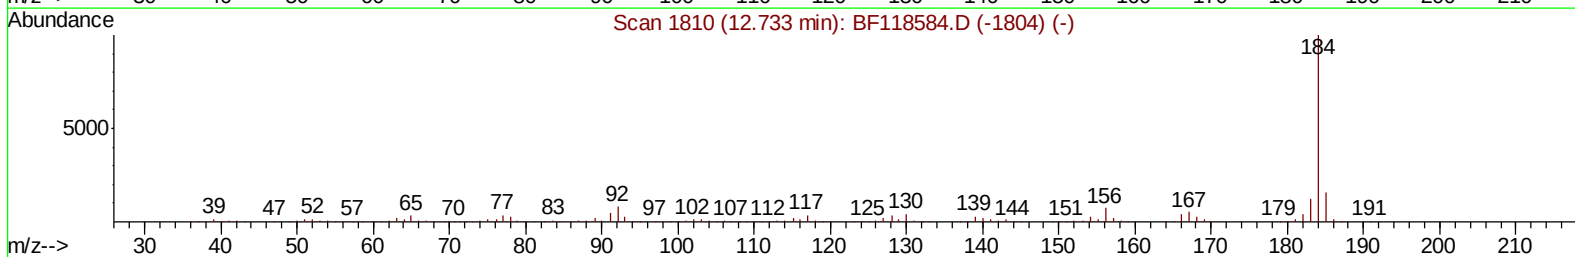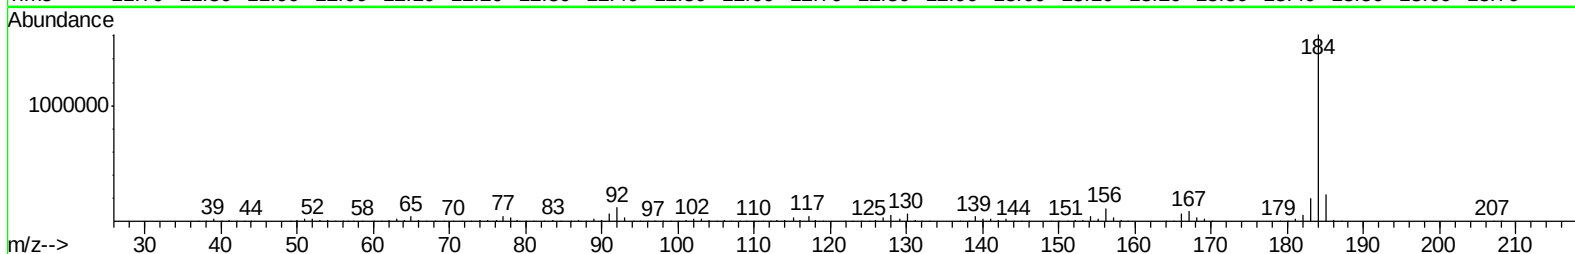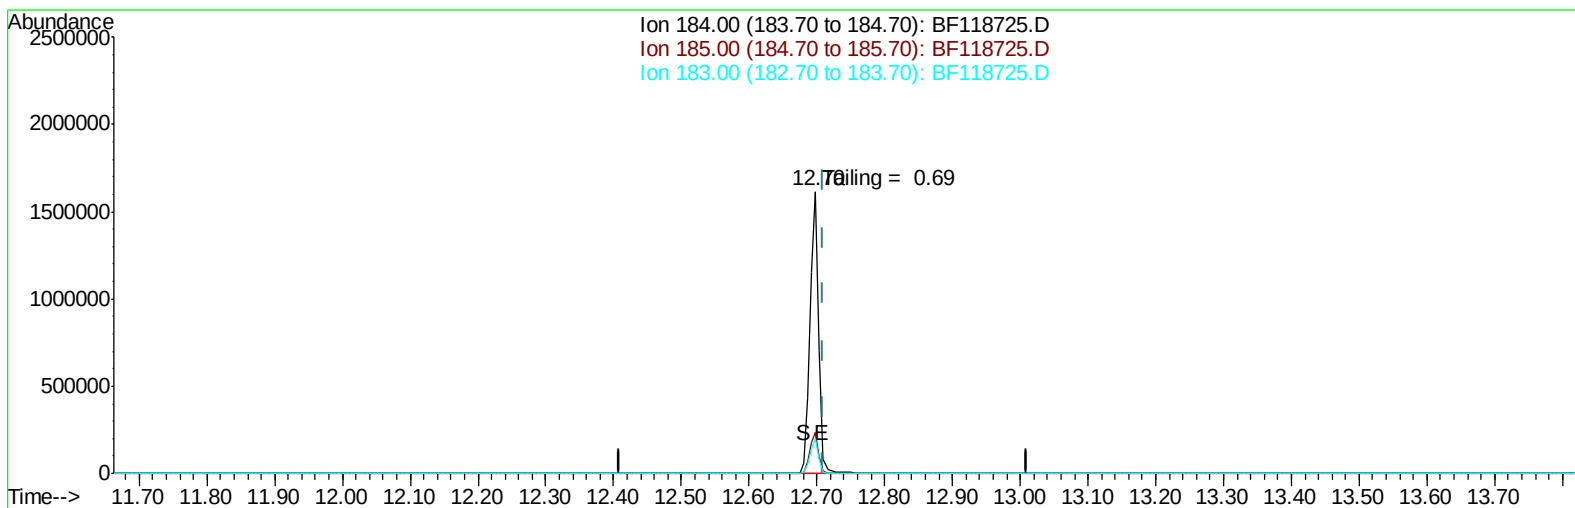

TIC: BF118725.D

(77) Benzidine

12.698min (-0.012) 0.00ng

response 1459281

Ion	Exp%	Act%
184.00	100	100
185.00	14.80	14.48
183.00	12.10	12.46
0.00	0.00	0.00