


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF012920\
 Data File : BF118725.D
 Acq On : 29 Jan 2020 11:41
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jan 27 14:24:10 2020

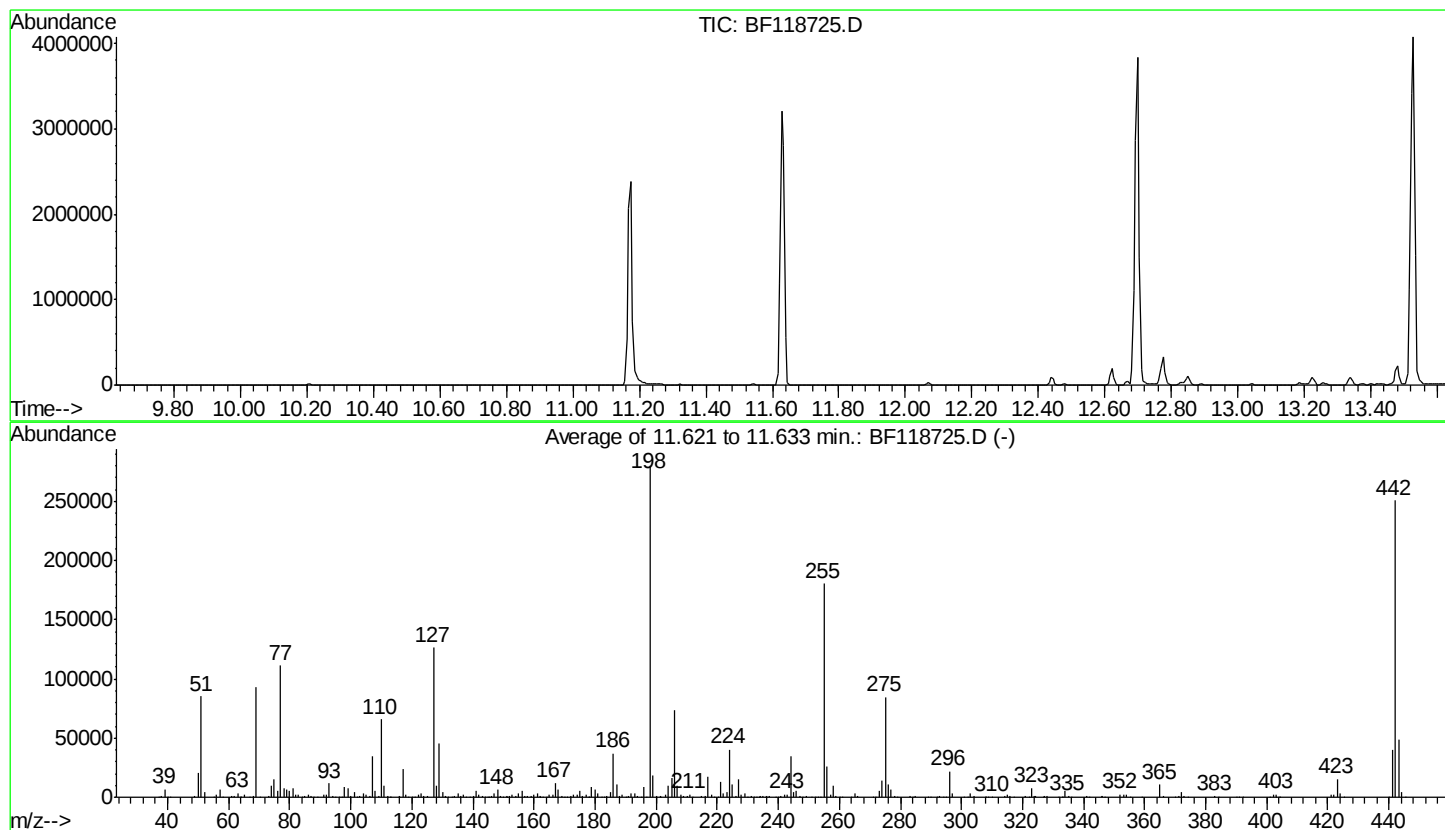

AutoFind: Scans 1621, 1622, 1623; Background Corrected with Scan 1616

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.4	85293	PASS
68	69	0.00	2	0.9	826	PASS
69	198	0.00	100	33.1	92842	PASS
70	69	0.00	2	0.5	440	PASS
127	198	10	80	45.1	126418	PASS
197	198	0.00	2	0.1	285	PASS
198	198	100	100	100.0	280298	PASS
199	198	5	9	6.7	18760	PASS
275	198	10	60	30.2	84602	PASS
365	198	1	100	3.7	10429	PASS
441	198	0.01	100	14.3	39989	PASS
442	198	50	100	89.4	250688	PASS
443	442	15	24	19.3	48423	PASS