
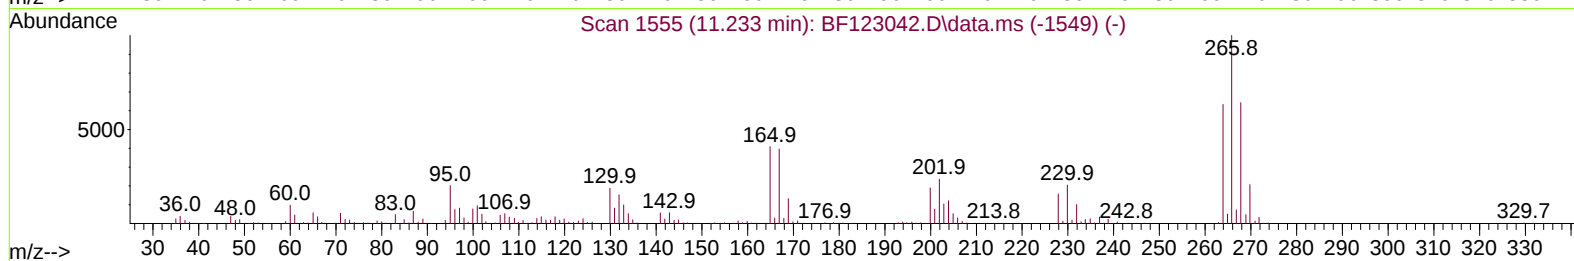
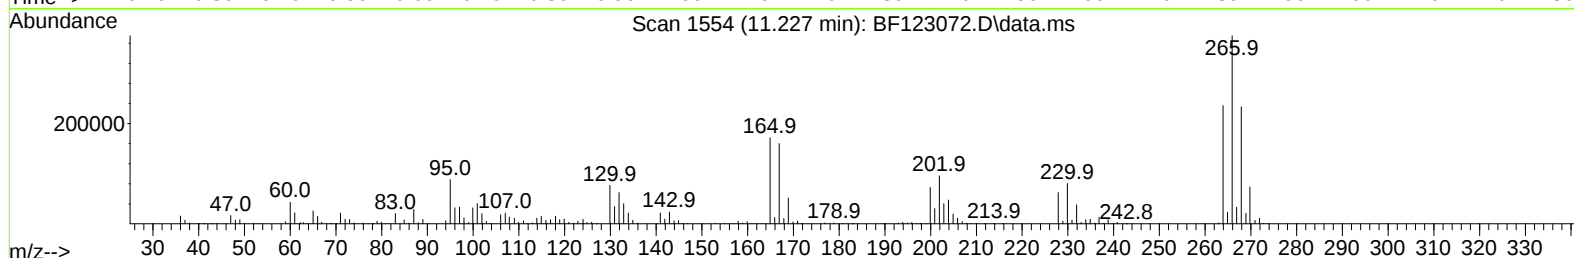


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012921\
Data File : BF123072.D
Acq On : 29 Jan 2021 9:39
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 30 01:29:01 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 29 12:29:00 2021
Response via : Initial Calibration

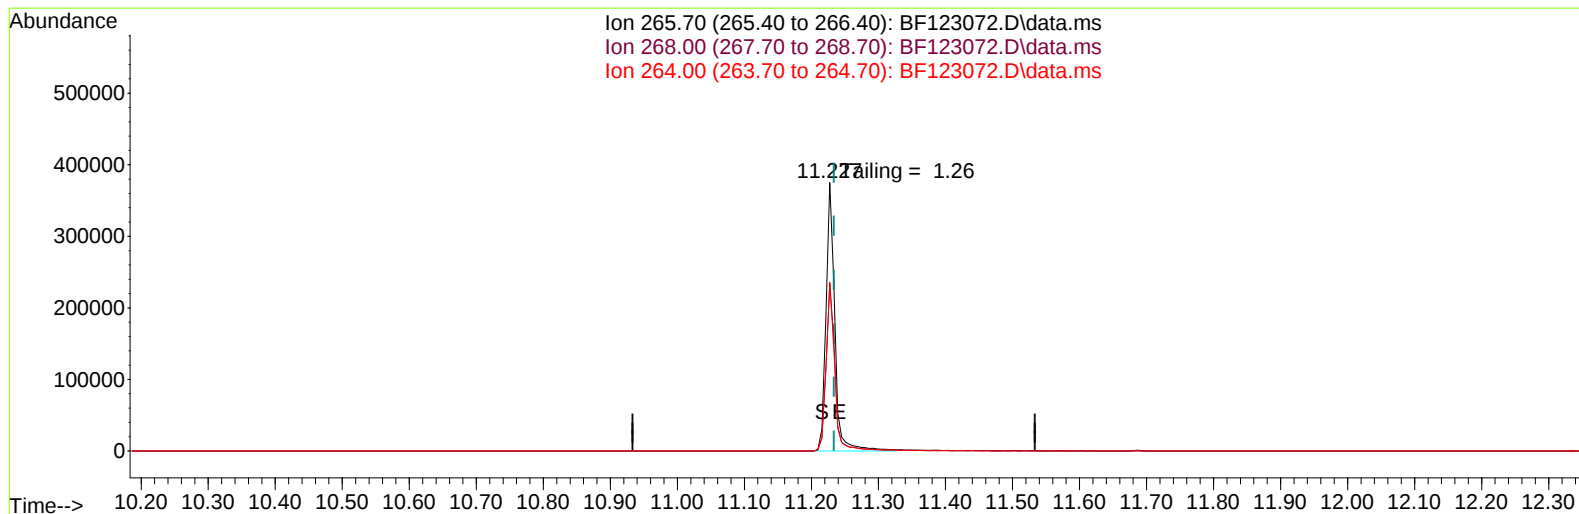

TIC: BF123072.D\data.ms

(70) Pentachlorophenol (C)




11.227min (-0.006) 36120.63 ng

response 344687

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	62.24
264.00	62.30	62.87
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012921\
 Data File : BF123072.D
 Acq On : 29 Jan 2021 9:39
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 30 01:29:01 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jan 29 12:29:00 2021
 Response via : Initial Calibration

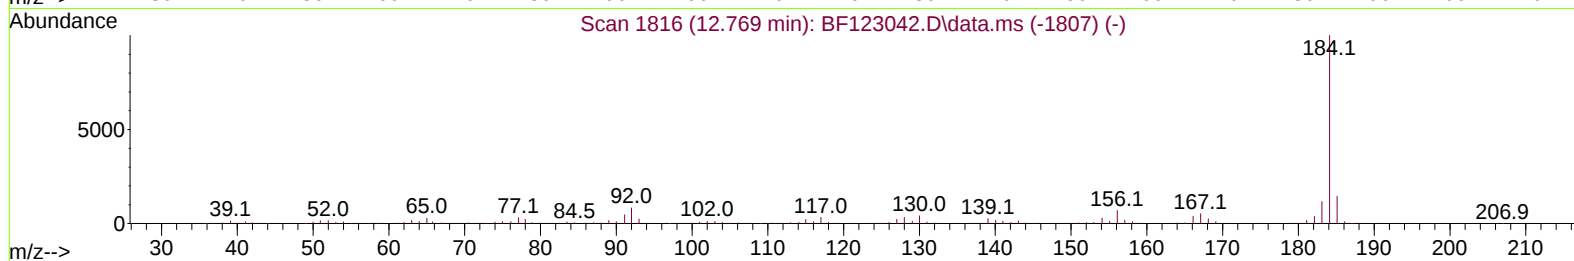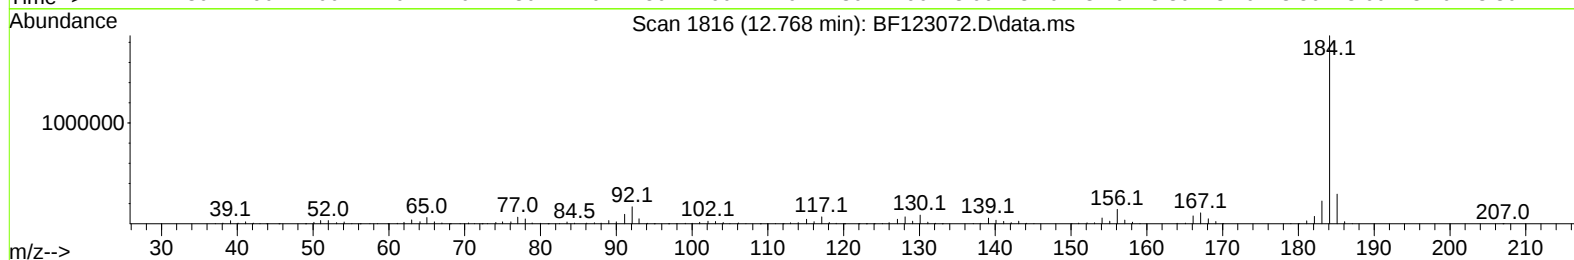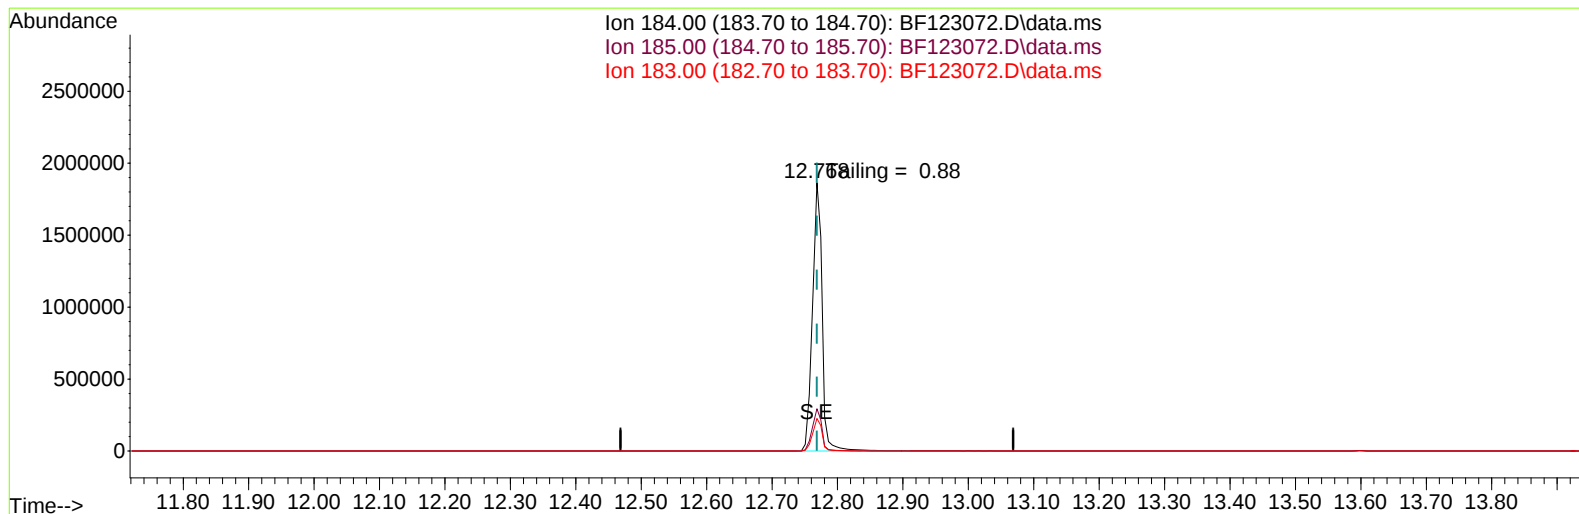

TIC: BF123072.D\data.ms

(77) Benzidine

12.768min (-0.000) 0.00 ng

response 1910014

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	15.74
183.00	12.10	12.12
0.00	0.00	0.00