
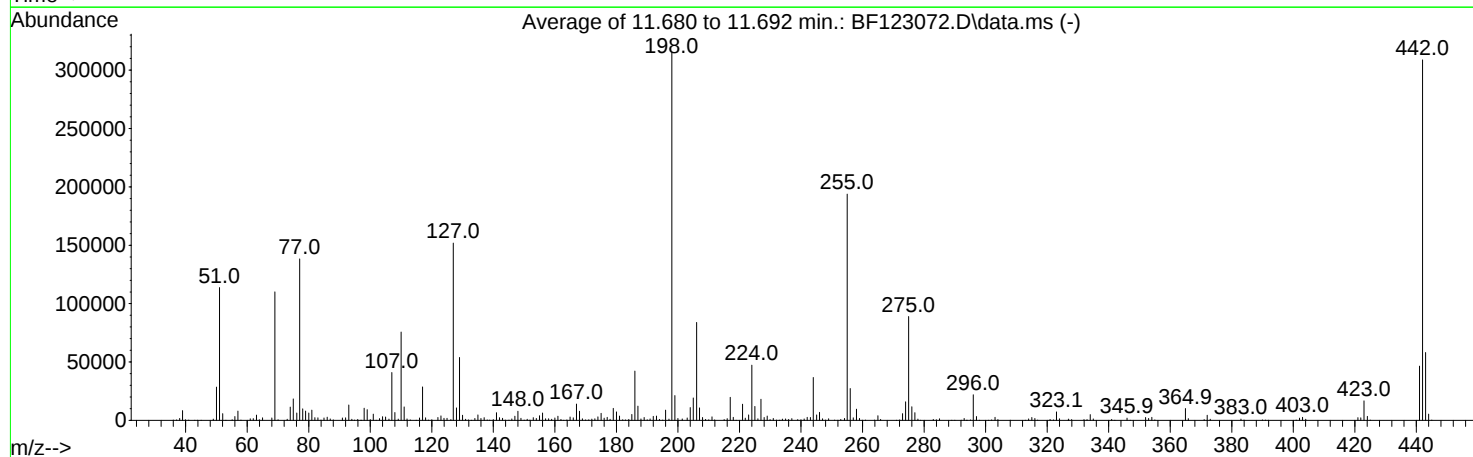


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012921\
 Data File : BF123072.D
 Acq On : 29 Jan 2021 9:39
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012721.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jan 29 12:29:00 2021

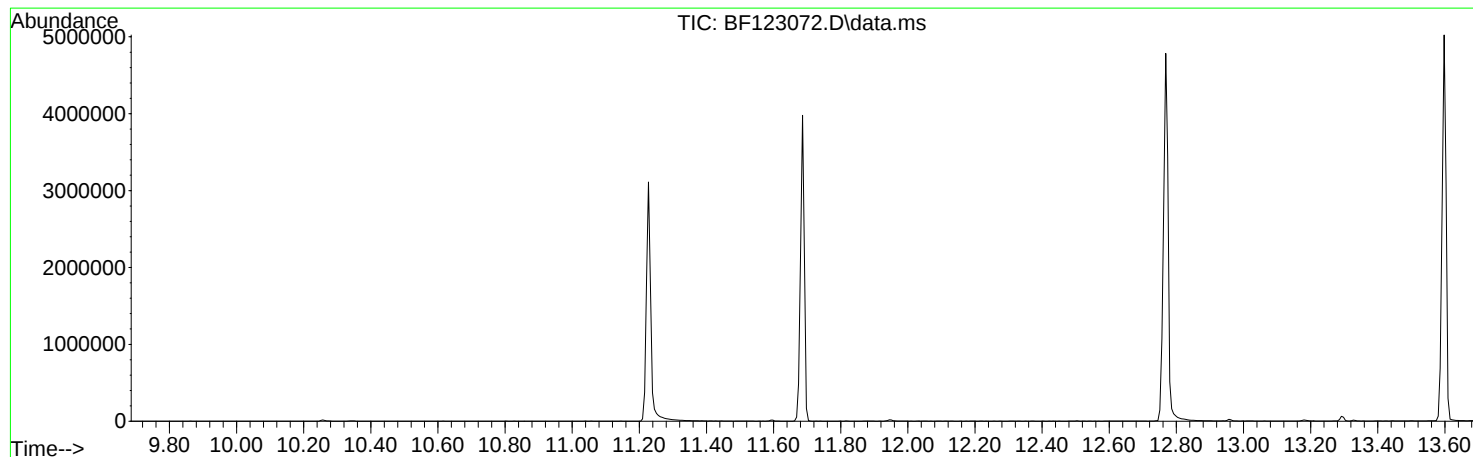

AutoFind: Scans 1631, 1632, 1633; Background Corrected with Scan 1625

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.1	113816	PASS
68	69	0.00	2	1.9	2143	PASS
69	198	0.00	100	34.9	110019	PASS
70	69	0.00	2	0.5	541	PASS
127	198	10	80	48.2	151883	PASS
197	198	0.00	2	0.3	1080	PASS
198	198	100	100	100.0	315136	PASS
199	198	5	9	6.7	21211	PASS
275	198	10	60	28.2	88989	PASS
365	198	1	100	3.2	10174	PASS
441	198	0.01	100	14.8	46496	PASS
442	442	50	100	100.0	308787	PASS
443	442	15	24	18.8	58109	PASS