
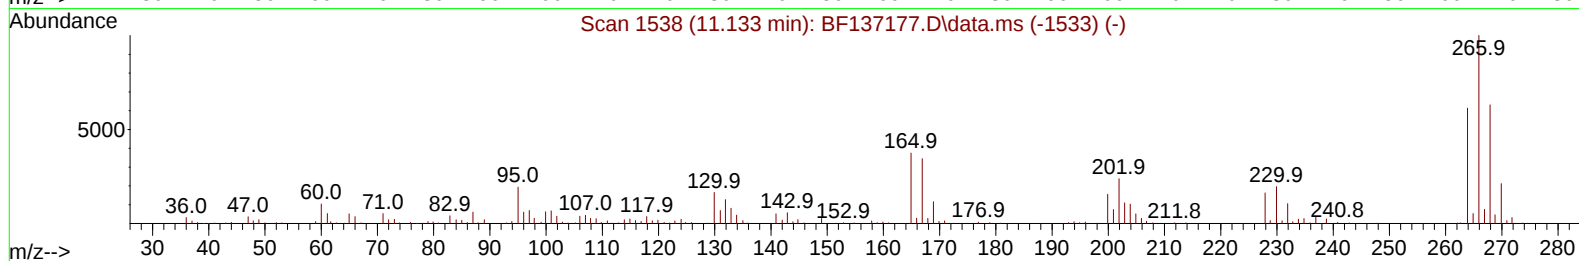
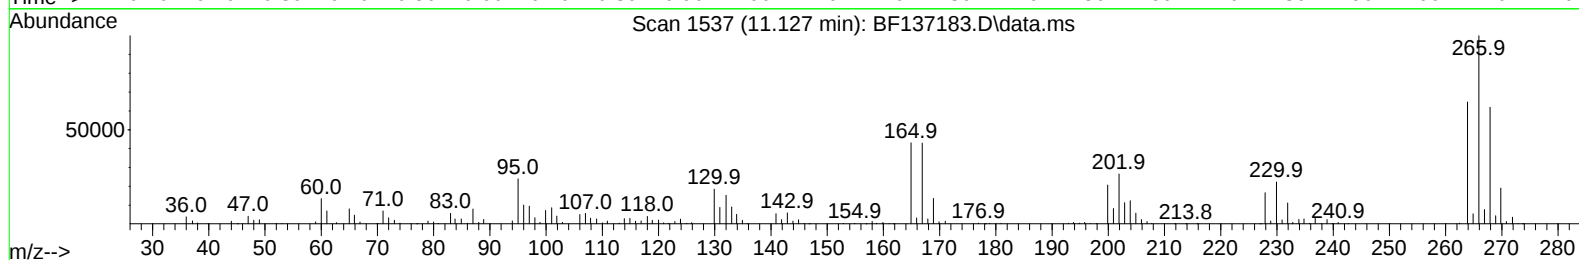


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012924\
Data File : BF137183.D
Acq On : 29 Jan 2024 10:05
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 29 11:26:57 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF012724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jan 27 02:14:33 2024
Response via : Initial Calibration

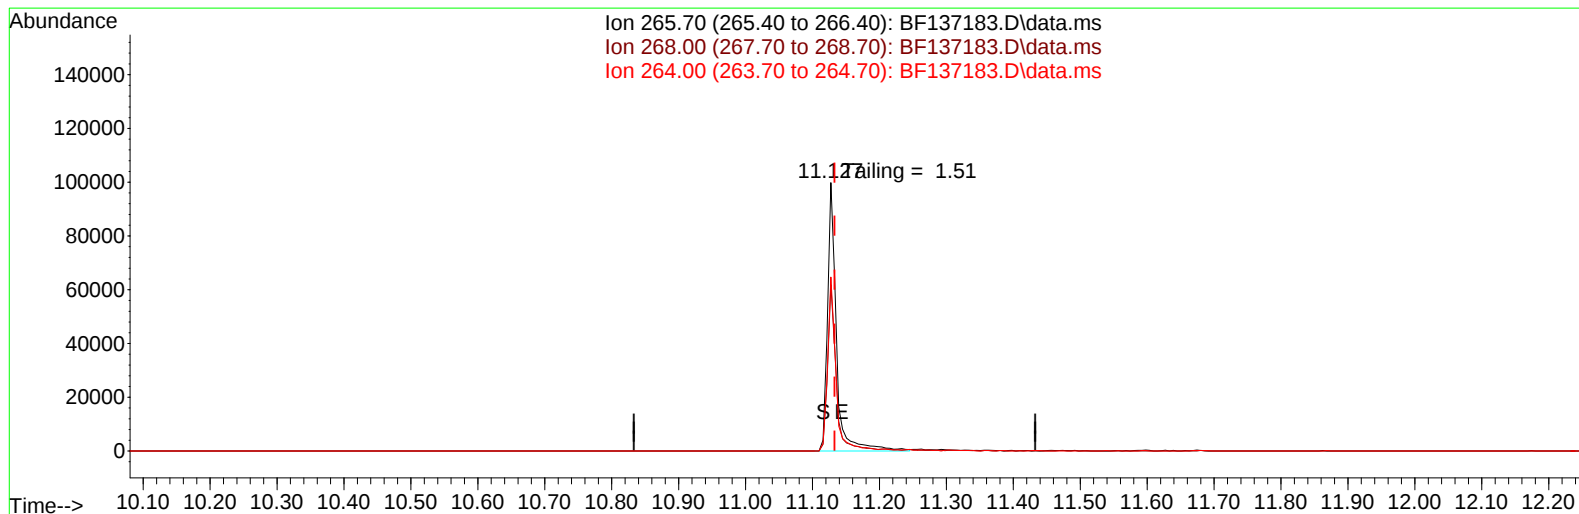

TIC: BF137183.D\data.ms

(70) Pentachlorophenol (C)




11.127min (-0.006) 24022.82 ng

response 93355

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.00	61.98
264.00	61.40	64.79
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012924\
Data File : BF137183.D
Acq On : 29 Jan 2024 10:05
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 29 11:26:57 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF012724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jan 27 02:14:33 2024
Response via : Initial Calibration

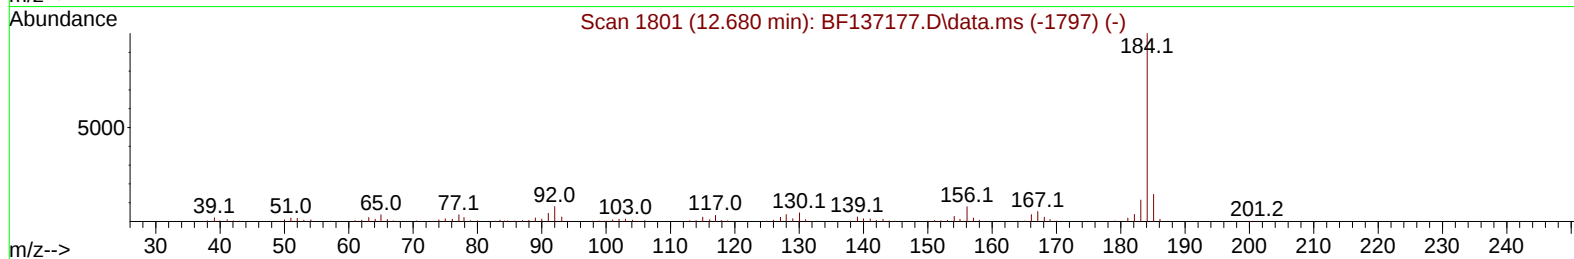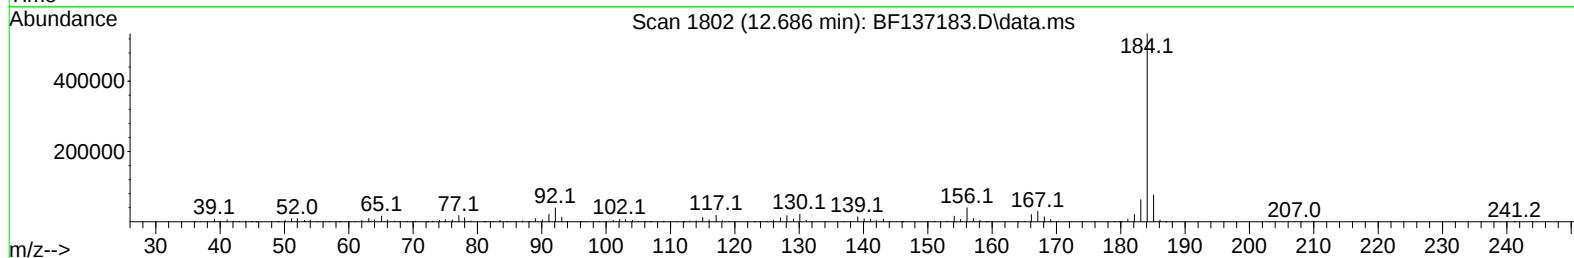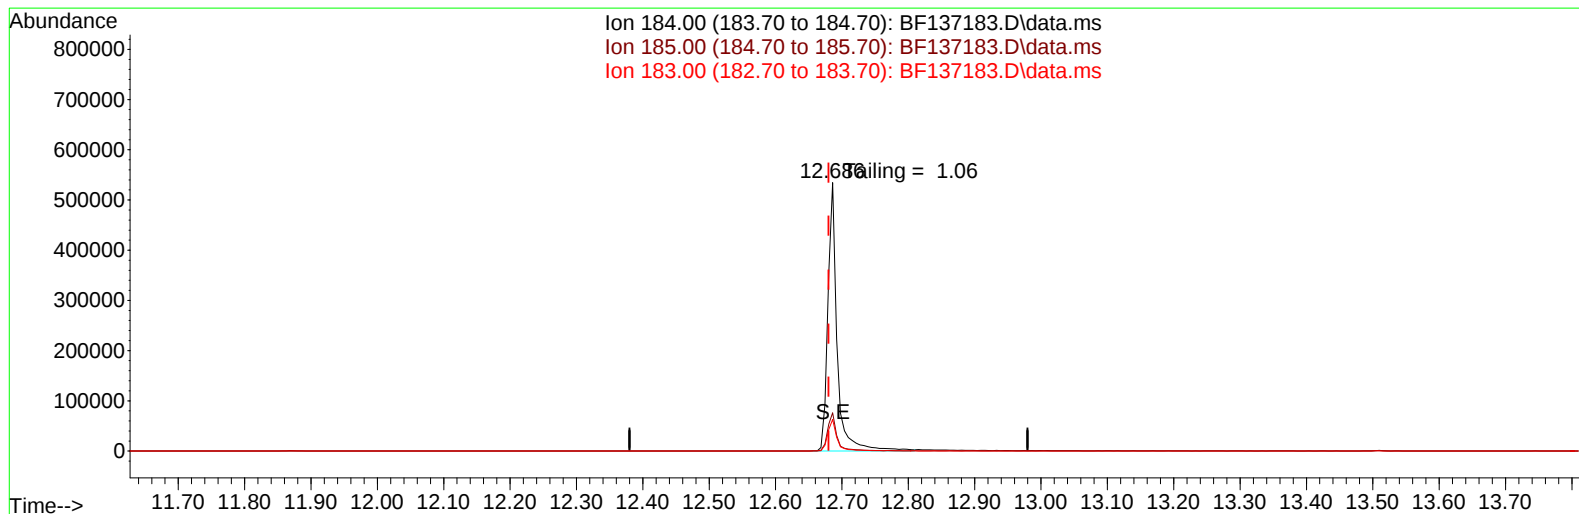

TIC: BF137183.D\data.ms

(77) Benzidine

12.686min (+ 0.006) 0.00 ng m

response 521452

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.25
183.00	11.50	11.76
0.00	0.00	0.00