

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012924\
Data File : BF137187.D
Acq On : 29 Jan 2024 12:02
Operator : CG\JU
Sample : PB158518BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB158518BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF012724.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF137187.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.205	12	20	28	rVB	677335	1565436	54.21%	9.639%
2	5.046	497	503	519	rBV	748225	956251	33.12%	5.888%
3	5.440	566	570	582	rBV	1431540	1347565	46.67%	8.298%
4	5.616	596	600	611	rVB2	55797	67954	2.35%	0.418%
5	6.051	671	674	683	rBV	77345	83986	2.91%	0.517%
6	6.428	734	738	757	rBV	1264299	1381272	47.84%	8.505%
7	6.798	798	801	808	rBV	395251	366832	12.70%	2.259%
8	6.951	823	827	837	rVB	139648	128380	4.45%	0.791%
9	7.363	892	897	909	rBV	1195973	1307318	45.27%	8.050%
10	8.075	1014	1018	1027	rBV	514788	496957	17.21%	3.060%
11	9.157	1197	1202	1205	rBV	2639173	2406881	83.35%	14.821%
12	9.834	1312	1317	1325	rBV	702340	597623	20.70%	3.680%
13	10.622	1447	1451	1466	rBV	1066266	991947	34.35%	6.108%
14	11.328	1567	1571	1588	rBV	670596	673873	23.34%	4.150%
15	12.933	1839	1844	1847	rBV	2847851	2887575	100.00%	17.781%
16	13.980	2018	2022	2032	rBV	609522	573481	19.86%	3.531%
17	15.468	2270	2275	2285	rBV	312119	406488	14.08%	2.503%




Sum of corrected areas: 16239819

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012924\
Data File : BF137187.D
Acq On : 29 Jan 2024 12:02
Operator : CG\JU
Sample : PB158518BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB158518BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF012724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

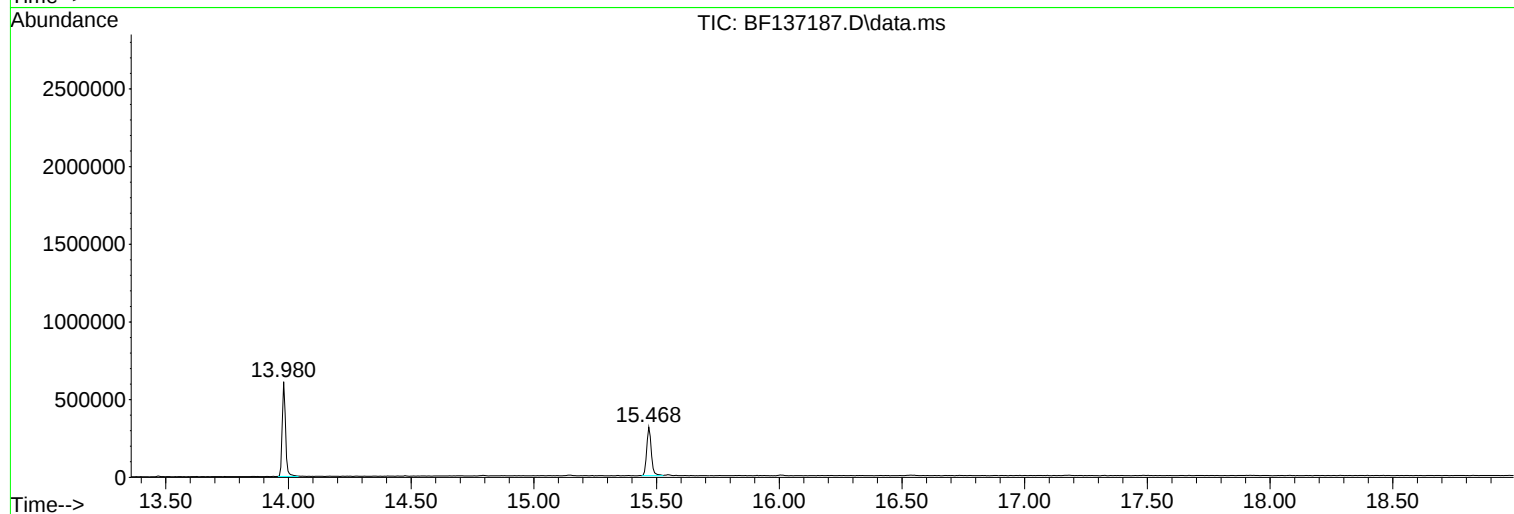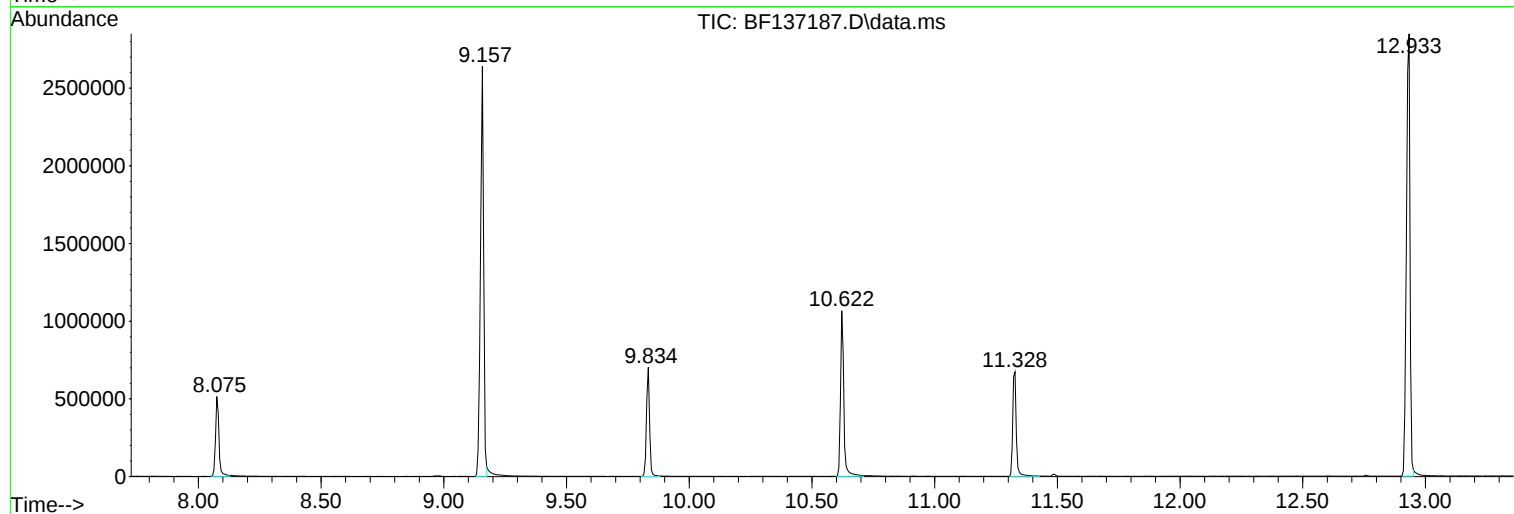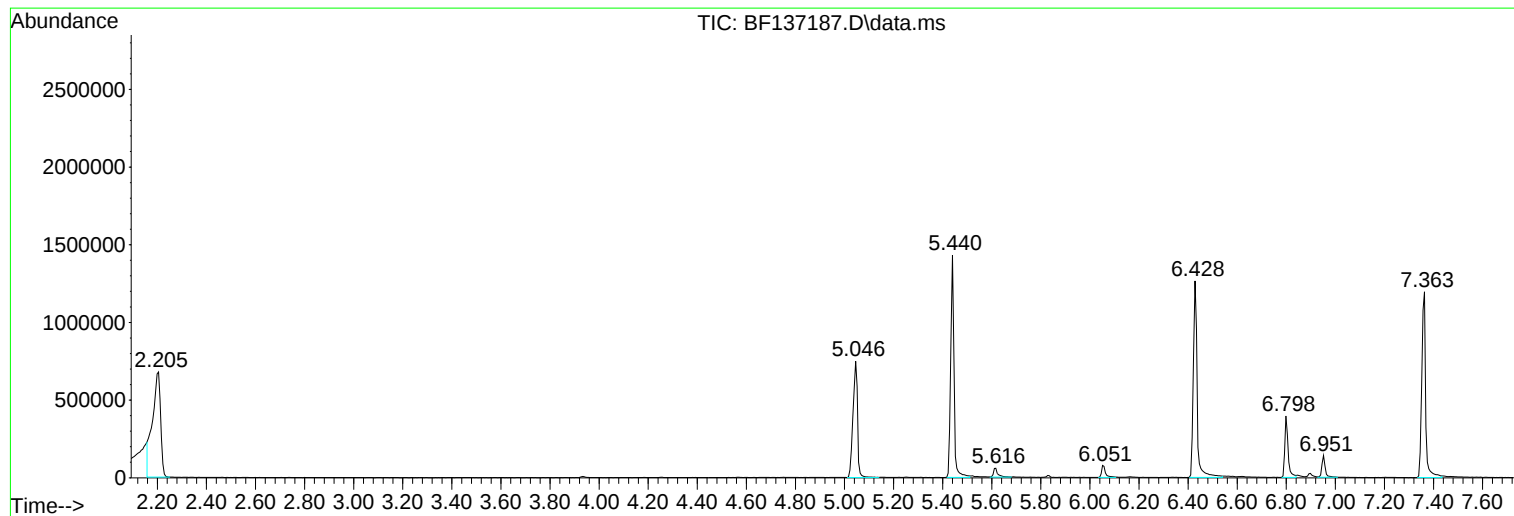

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012924\
Data File : BF137187.D
Acq On : 29 Jan 2024 12:02
Operator : CG\JU
Sample : PB158518BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB158518BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF012724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012924\
Data File : BF137187.D
Acq On : 29 Jan 2024 12:02
Operator : CG\JU
Sample : PB158518BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB158518BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF012724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------