


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012924\
Data File : BF137183.D
Acq On : 29 Jan 2024 10:05
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF012724.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Sat Jan 27 02:14:33 2024

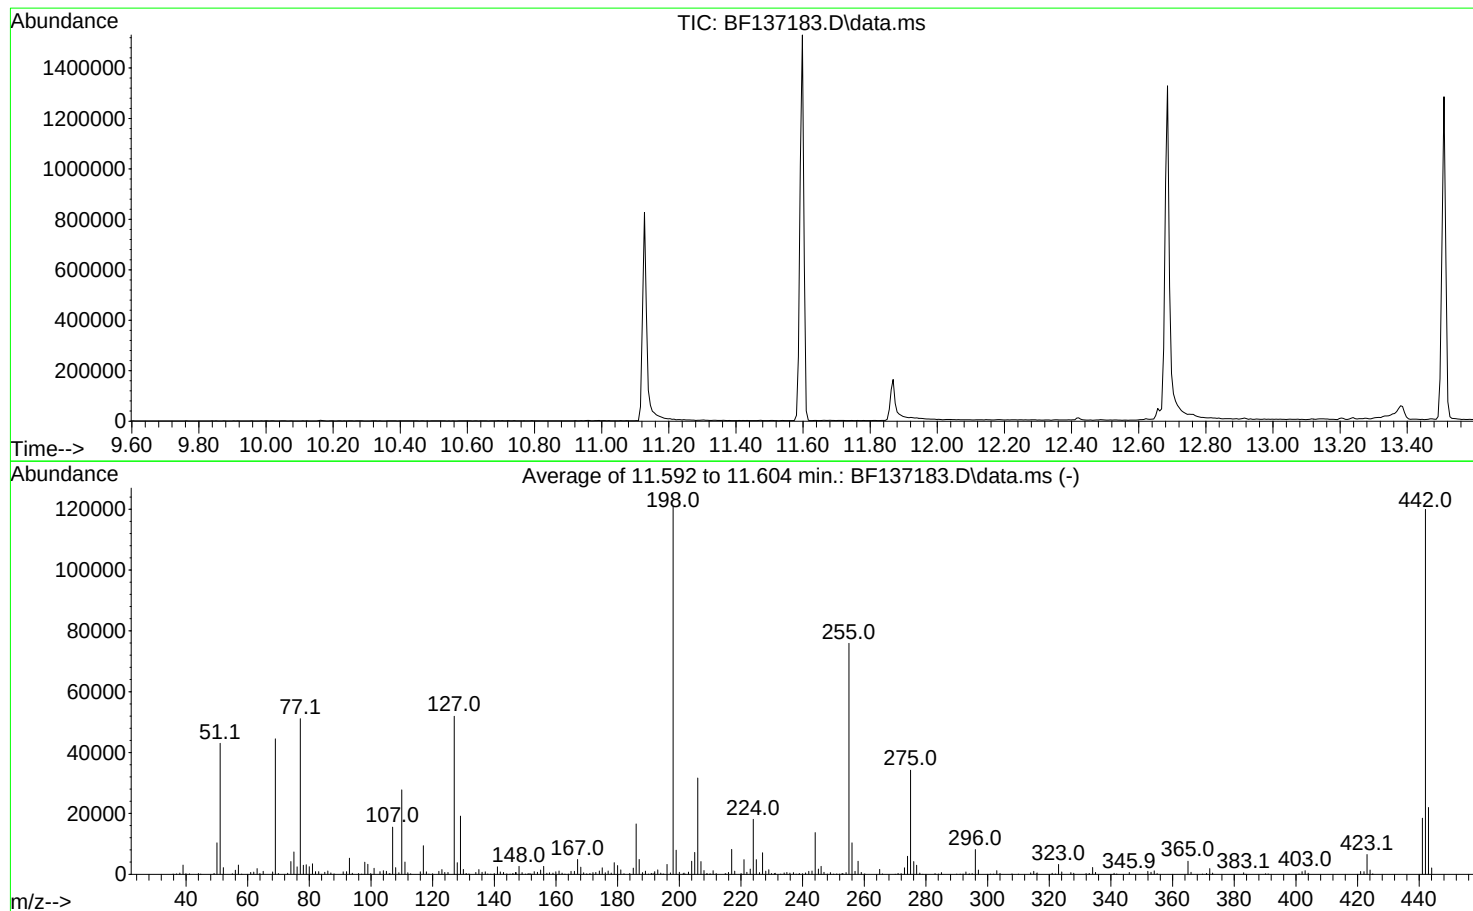




AutoFind: Scans 1616, 1617, 1618; Background Corrected with Scan 1610

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.6	43036	PASS
68	69	0.00	2	1.7	763	PASS
69	198	0.00	100	36.8	44496	PASS
70	69	0.00	2	0.5	212	PASS
127	198	10	80	43.0	51933	PASS
197	198	0.00	2	0.4	430	PASS
198	198	100	100	100.0	120901	PASS
199	198	5	9	6.6	7937	PASS
275	198	10	60	28.3	34219	PASS
365	198	1	100	3.5	4266	PASS
441	198	0.01	100	15.3	18455	PASS
442	442	50	100	100.0	119901	PASS
443	442	15	24	18.3	21953	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012924\
Data File : BF137183.D
Acq On : 29 Jan 2024 10:05
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jan 29 11:26:57 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF012724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jan 27 02:14:33 2024
Response via : Initial Calibration

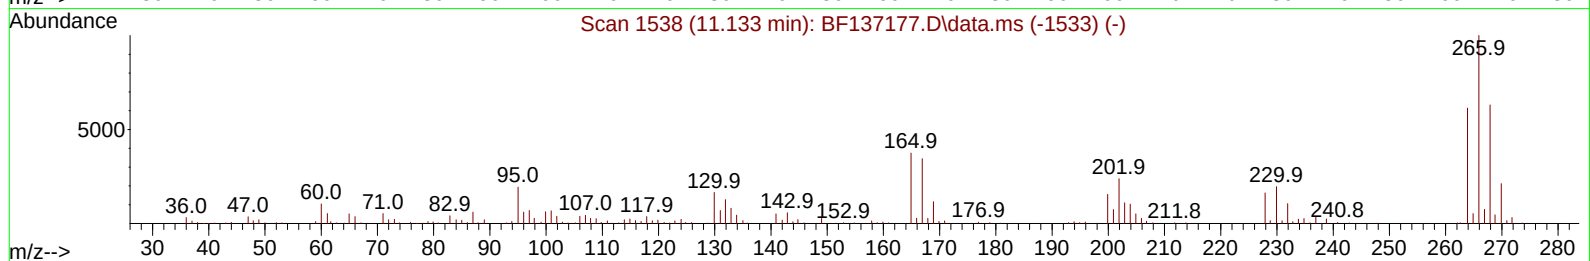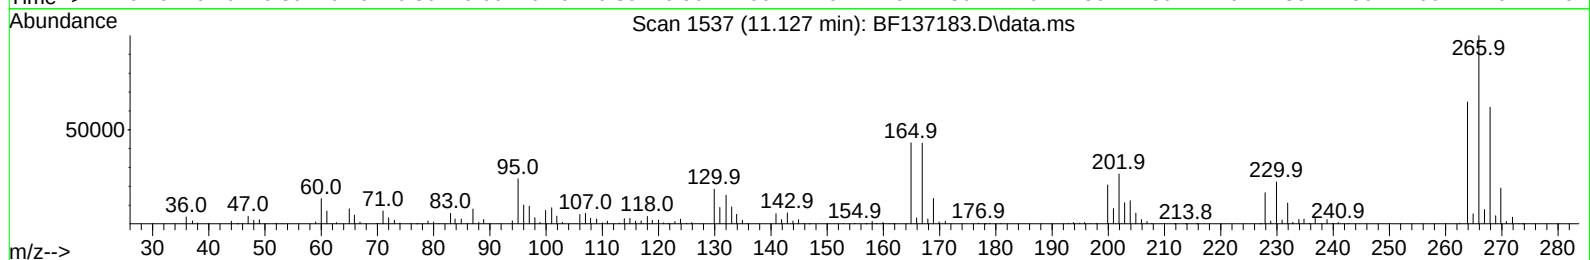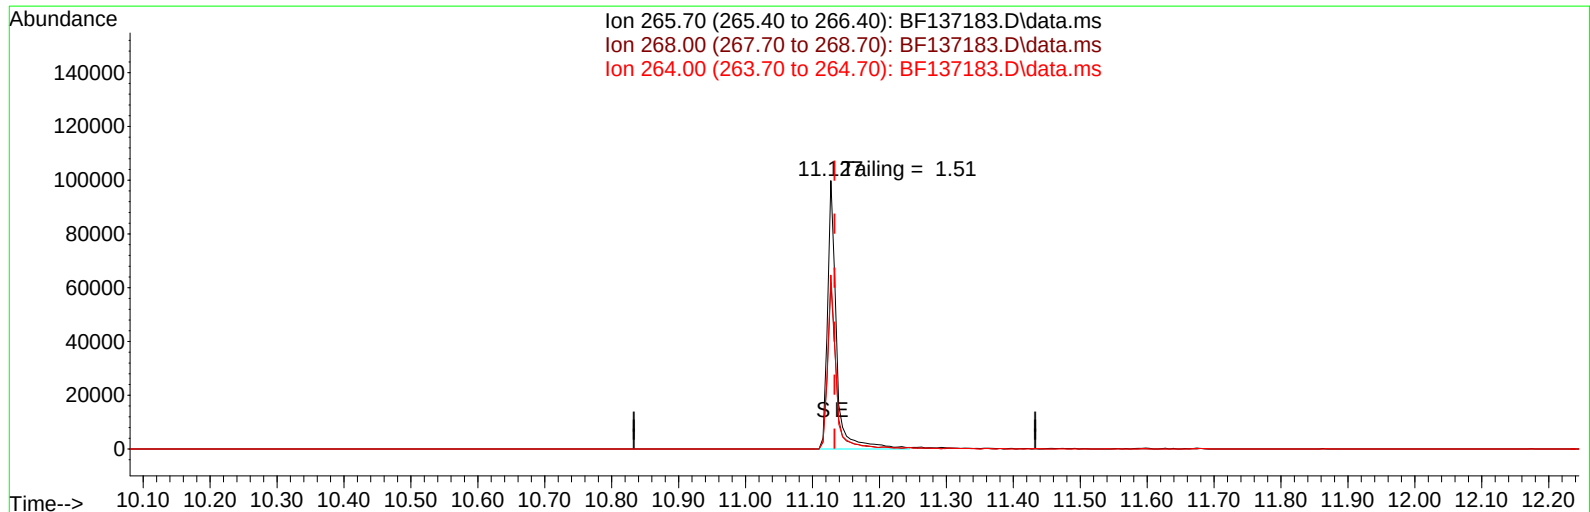

TIC: BF137183.D\data.ms

(70) Pentachlorophenol (C)

11.127min (-0.006) 24022.82 ng




response 93355

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.00	61.98
264.00	61.40	64.79
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012924\
Data File : BF137183.D
Acq On : 29 Jan 2024 10:05
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jan 29 11:26:57 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF012724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jan 27 02:14:33 2024
Response via : Initial Calibration

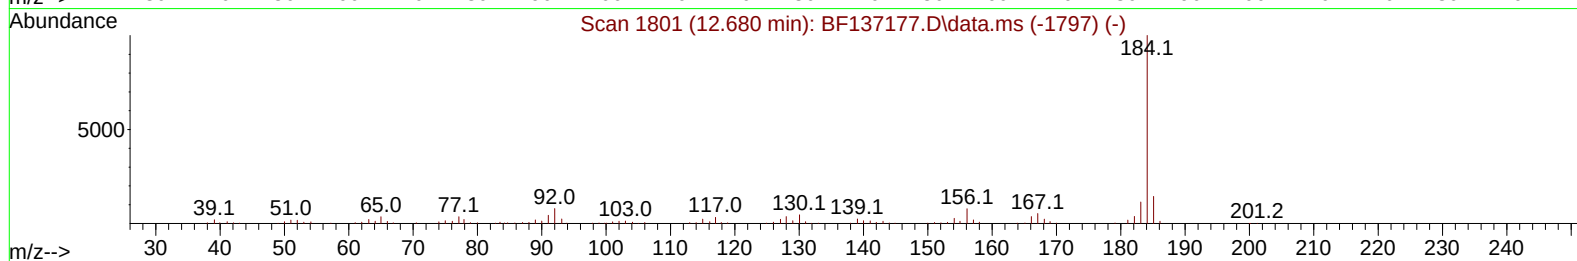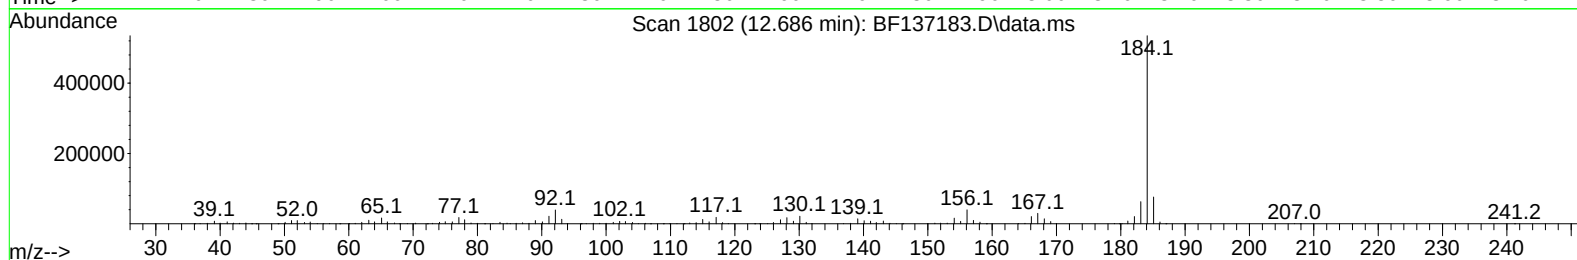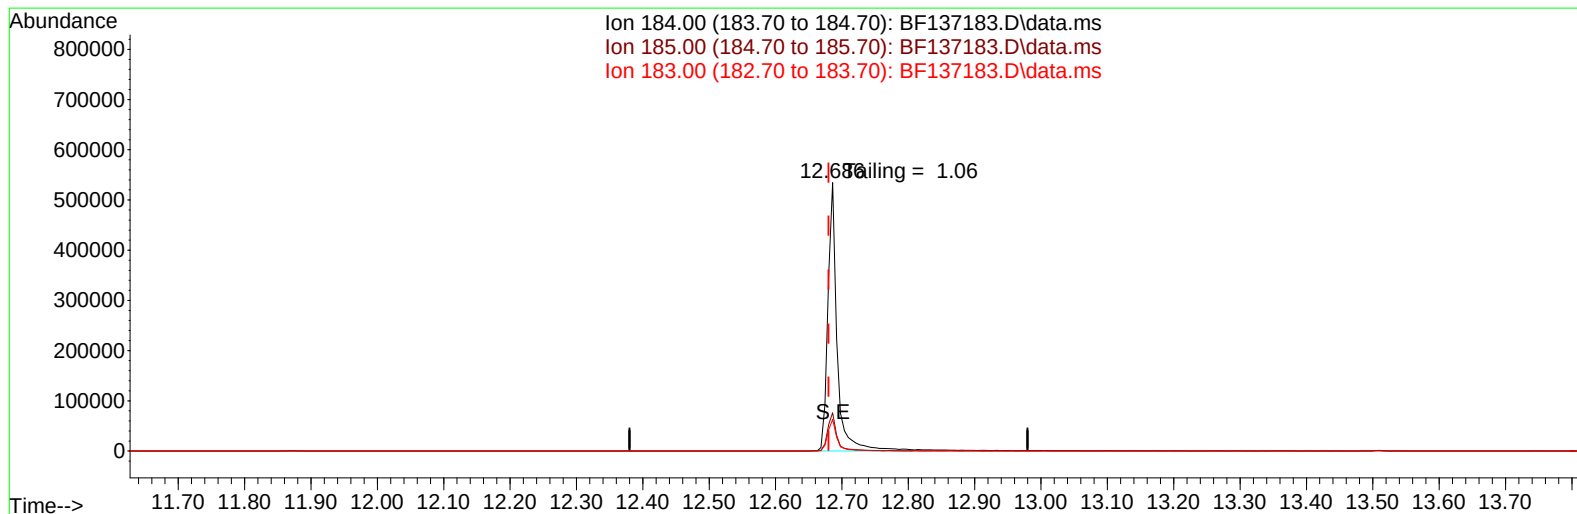

TIC: BF137183.D\data.ms

(77) Benzidine

12.686min (+ 0.006) 0.00 ng m

response 521452

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.25
183.00	11.50	11.76
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
1/29/2024	BNA_F	<u>BF137183.D</u>
Compound Name	Response	Retention Time
DDT	182167	13.51
DDD	3022	13.239
DDE	0	12.88
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3022	185189	1.63

Instrument :
BNA_F
ClientSampleId :
DFTPP