
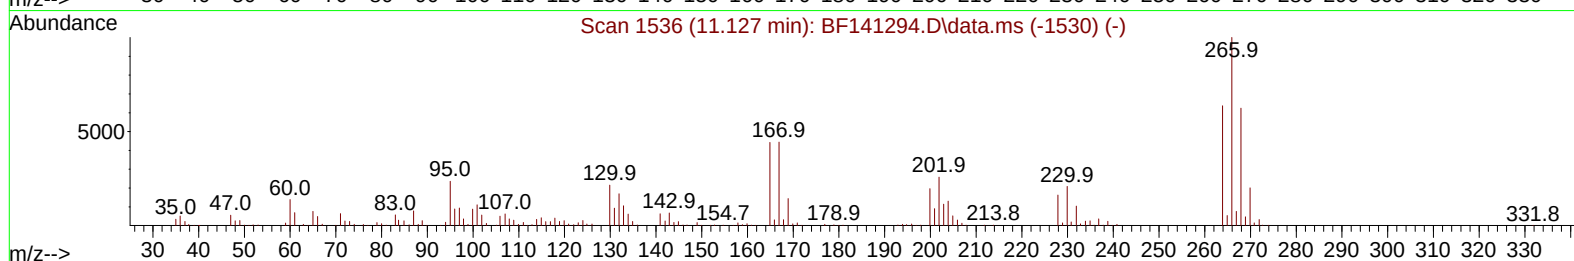
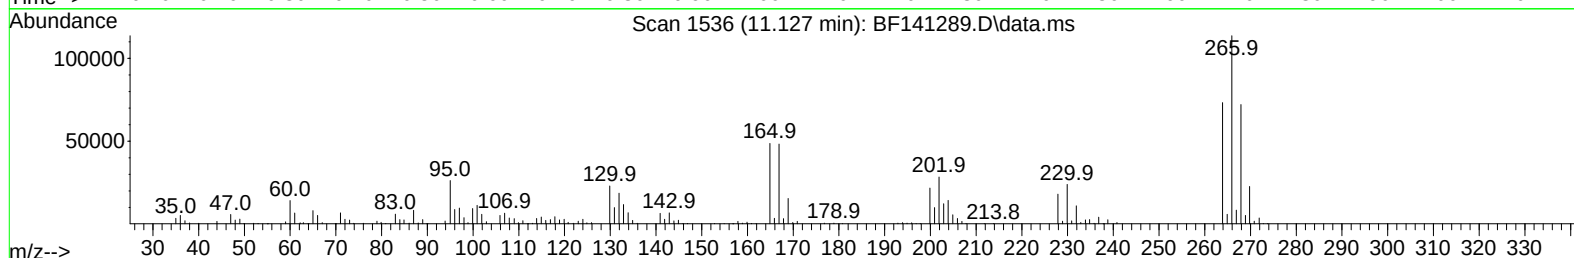


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012925\
Data File : BF141289.D
Acq On : 29 Jan 2025 10:03
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 29 13:18:12 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF012925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 29 13:12:40 2025
Response via : Initial Calibration

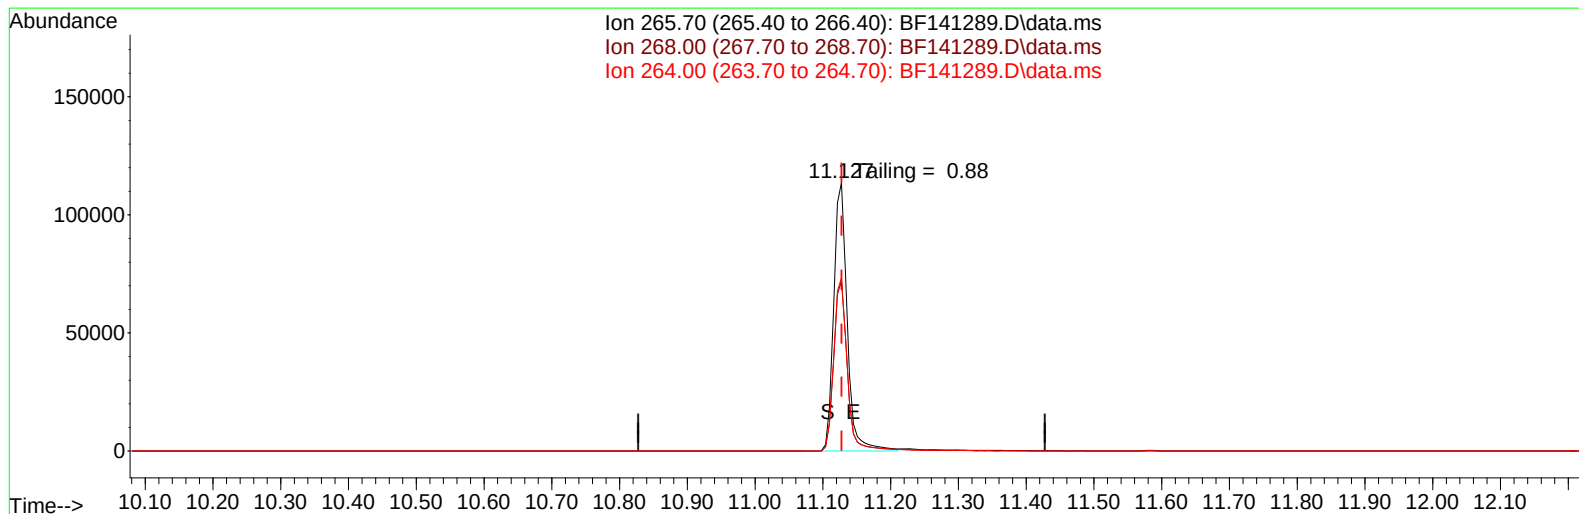

TIC: BF141289.D\data.ms

(70) Pentachlorophenol (C)




11.127min (-0.000) 18353.04 ng

response 157302

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	68.00	63.47
264.00	63.20	64.50
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012925\
Data File : BF141289.D
Acq On : 29 Jan 2025 10:03
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 29 13:18:12 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF012925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 29 13:12:40 2025
Response via : Initial Calibration

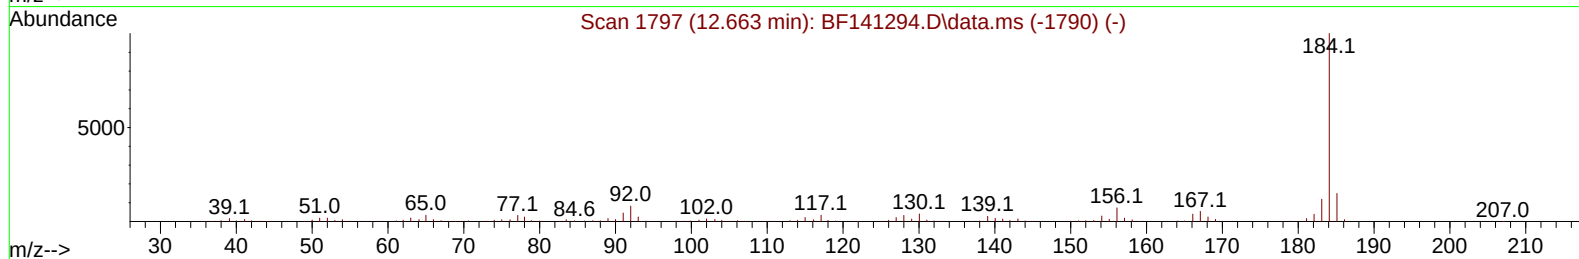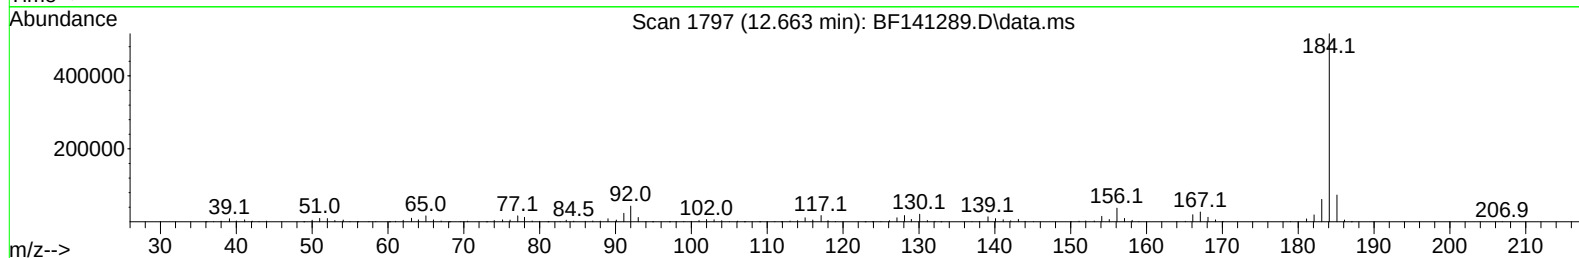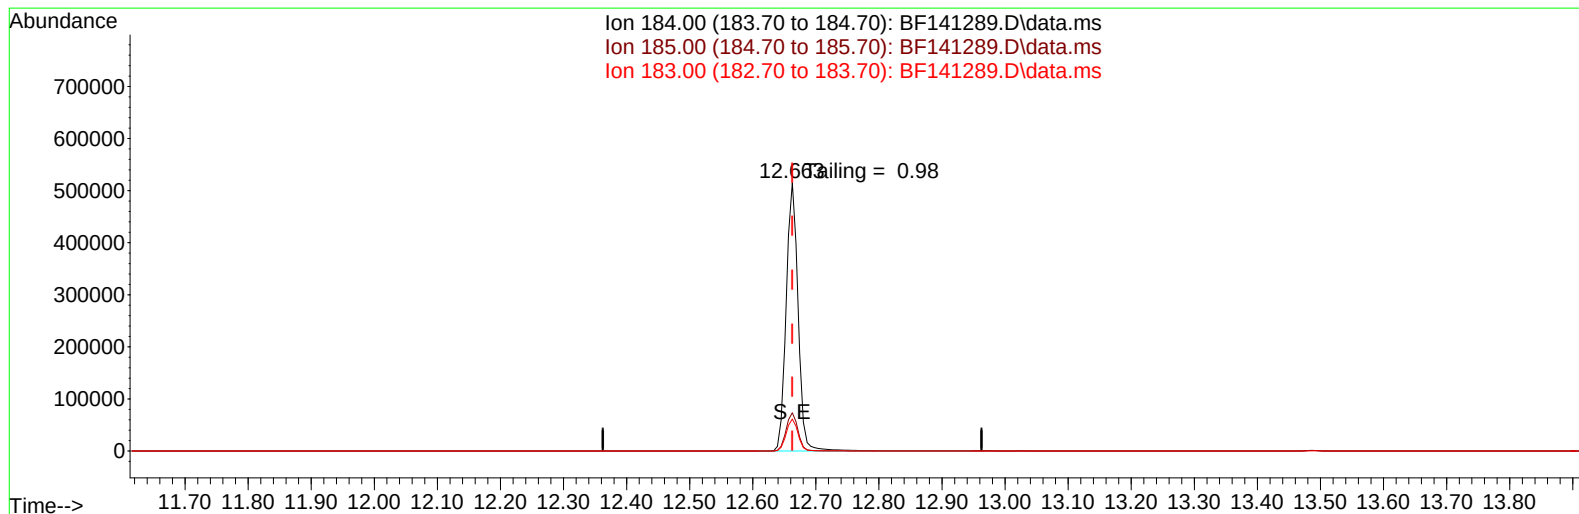

TIC: BF141289.D\data.ms

(77) Benzidine**12.663min (-0.000) 86413.53 ng****response 677498**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.27
183.00	11.70	11.93
0.00	0.00	0.00