


Data Path : Z:\HPCHEM1\BNA F\Data\BF013015\
 Data File : BF077145.D
 Acq On : 30 Jan 2015 10:07
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF011415.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jan 28 16:07:35 2015

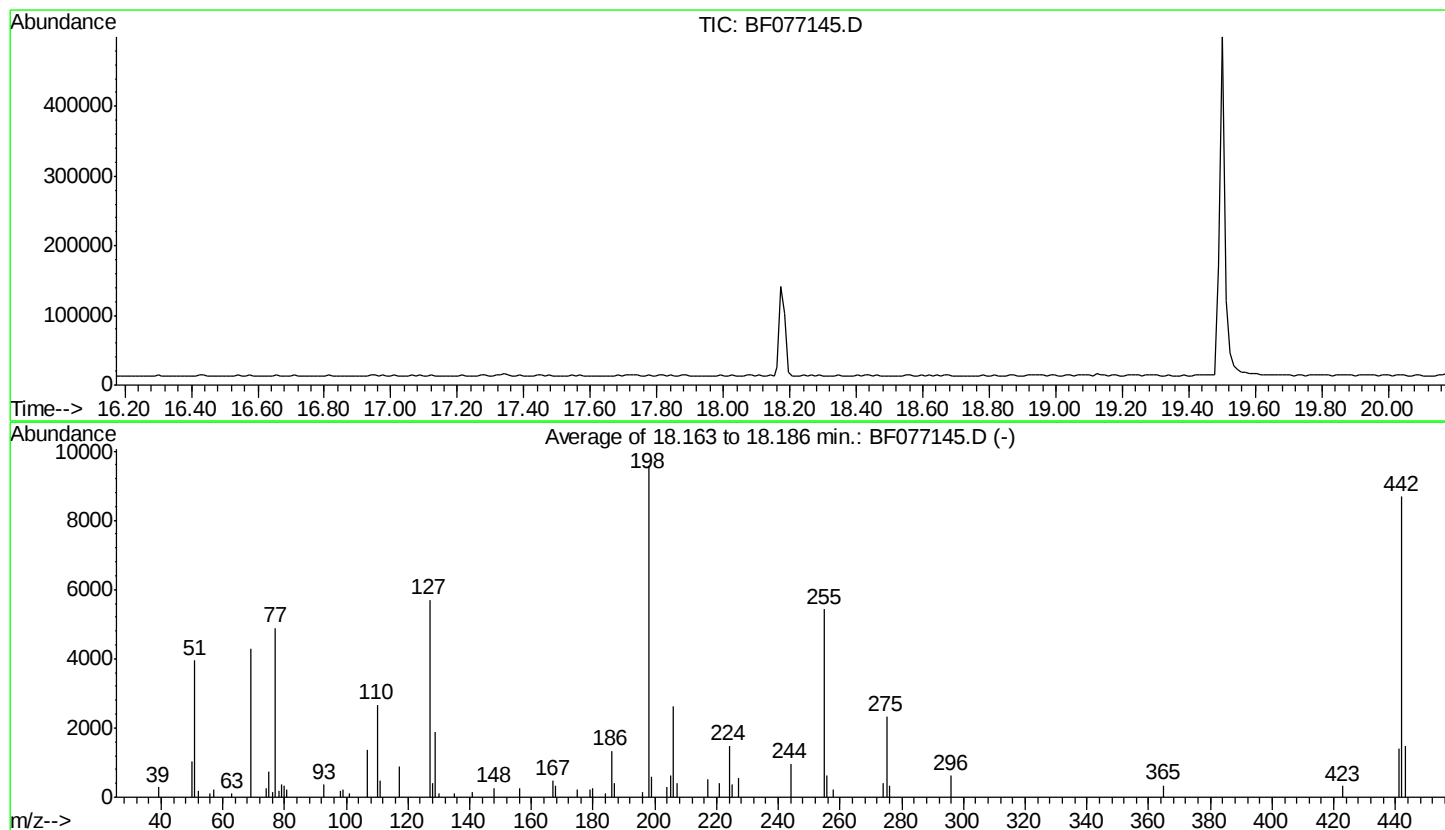

AutoFind: Scans 1494, 1495, 1496; Background Corrected with Scan 1491

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.2	3942	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	44.9	4304	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	59.5	5703	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	9577	PASS
199	198	5	9	6.1	580	PASS
275	198	10	60	24.3	2329	PASS
365	198	1	100	3.7	351	PASS
441	442	0.01	24	16.1	1400	PASS
442	198	50	100	90.6	8680	PASS
443	442	15	24	17.2	1493	PASS