

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF013015\
 Data File : BF077147.D
 Acq On : 30 Jan 2015 15:15
 Operator : TP/IZ
 Sample : PB81569BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB81569BL

Quant Time: Jan 30 22:28:10 2015
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF011415.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jan 30 22:20:35 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.68	152	25756	20.00	ng	0.00
21) Naphthalene-d8	10.59	136	112139	20.00	ng	0.00
38) Acenaphthene-d10	14.72	164	59802	20.00	ng	0.00
63) Phenanthrene-d10	17.57	188	106876	20.00	ng	0.00
75) Chrysene-d12	21.17	240	112786	20.00	ng	0.00
86) Perylene-d12	23.17	264	100612	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	4.70	112	185485	118.41	ng	0.00
7) Phenol-d6	7.09	99	226819	114.78	ng	0.00
23) Nitrobenzene-d5	8.99	82	139859	69.10	ng	0.00
41) 2,4,6-Tribromophenol	16.45	330	52780	108.73	ng	0.00
44) 2-Fluorobiphenyl	13.25	172	290266	73.87	ng	0.00
78) Terphenyl-d14	19.83	244	337543	68.90	ng	0.00


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF013015\
Data File : BF077147.D
Acq On : 30 Jan 2015 15:15
Operator : TP/IZ
Sample : PB81569BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB81569BL

Quant Time: Jan 30 22:28:10 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF011415.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 30 22:20:35 2015
Response via : Initial Calibration

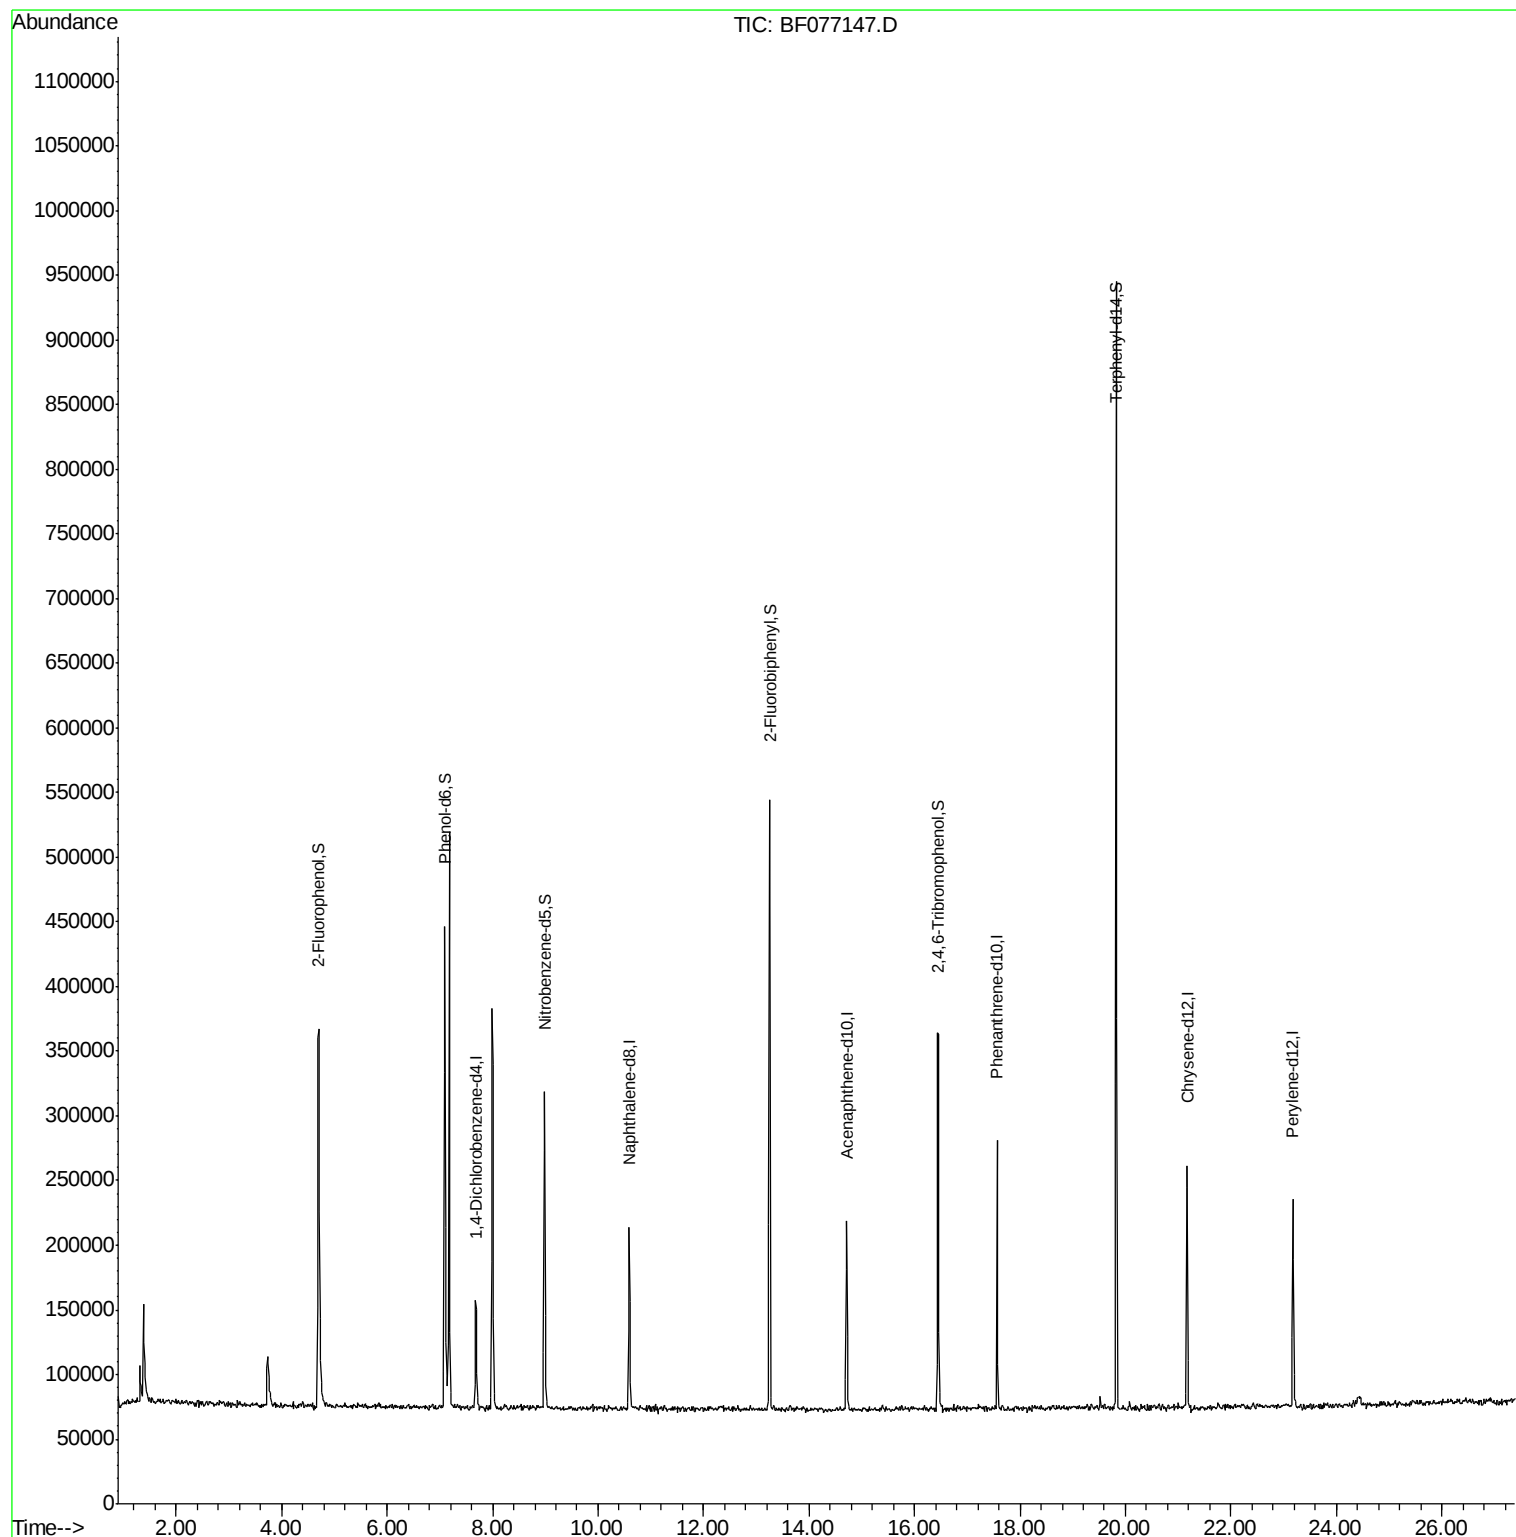

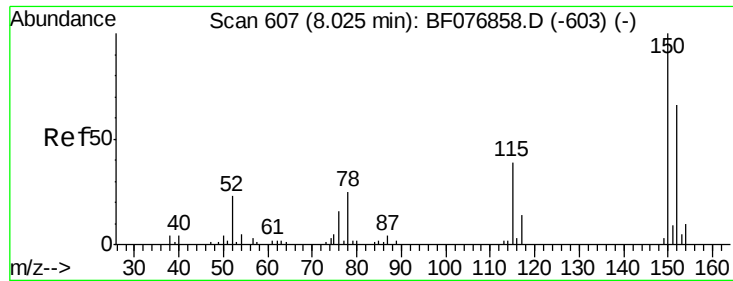


#1




1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 7.68 min Scan# 594
Delta R.T. 0.00 min
Lab File: BF077147.D
Acq: 30 Jan 2015 15:15

Instrument :
BNA_F
ClientSampleId :
PB81569BL

Tgt Ion:152 Resp: 25756
Ion Ratio Lower Upper
152 100
150 155.2 121.7 182.5
115 68.3 47.0 70.6

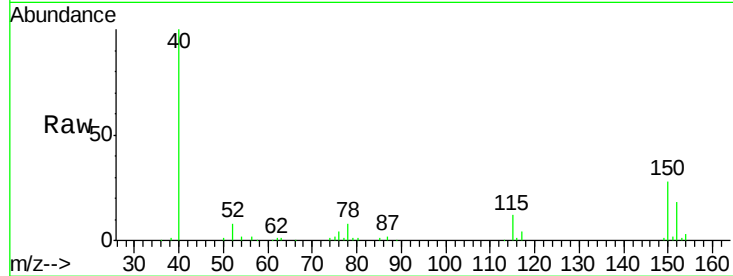


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

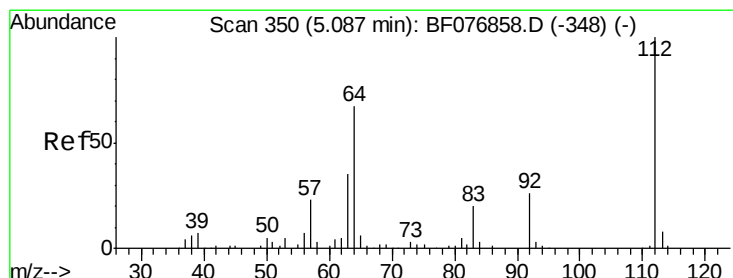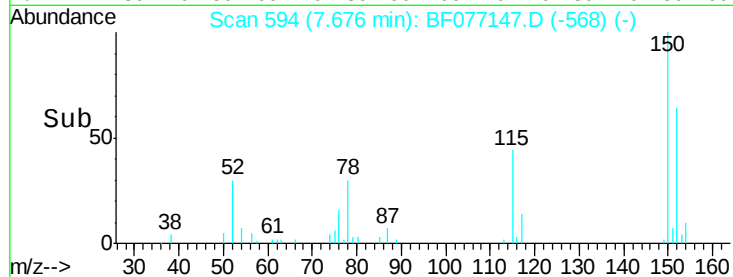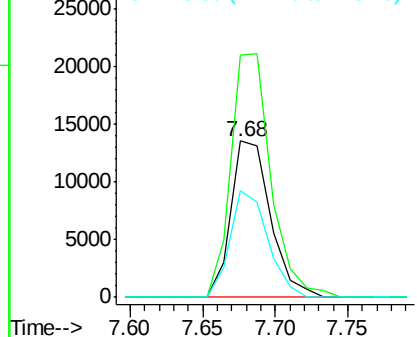



#5

2-Fluorophenol
Concen: 118.41 ng
RT: 4.70 min Scan# 334
Delta R.T. 0.00 min
Lab File: BF077147.D
Acq: 30 Jan 2015 15:15

Tgt Ion:112 Resp: 185485
Ion Ratio Lower Upper
112 100
64 64.2 54.2 81.4
63 34.9 28.4 42.6

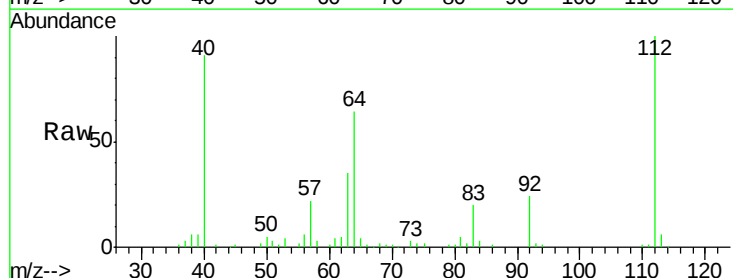

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF0
Ion 63.00 (62.70 to 63.70): BF0

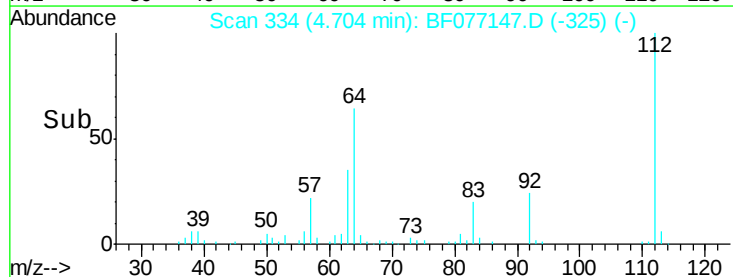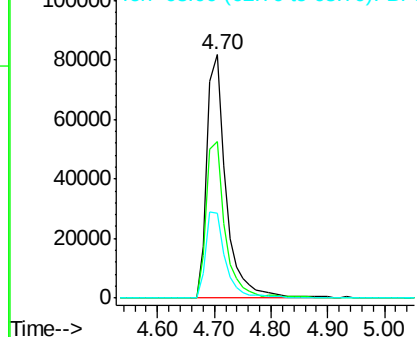



#7

Phenol-d6

Concen: 114.78 ng

RT: 7.09 min Scan# 543

Delta R.T. 0.00 min

Lab File: BF077147.D

Acq: 30 Jan 2015 15:15

Instrument :

BNA_F

ClientSampleId :

PB81569BL


Tgt Ion: 99 Resp: 226819

Ion Ratio Lower Upper

99 100

42 17.7 15.0 22.4




71 37.6 30.5 45.7

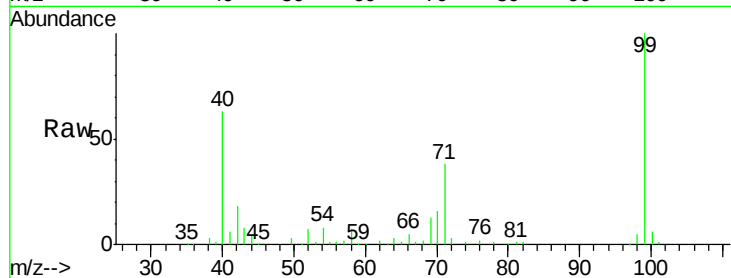

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

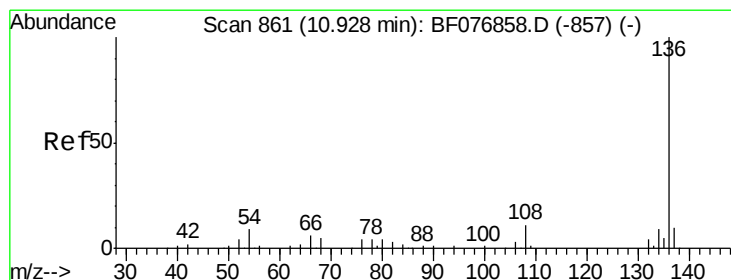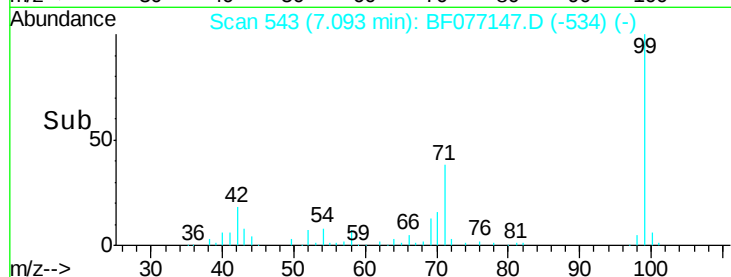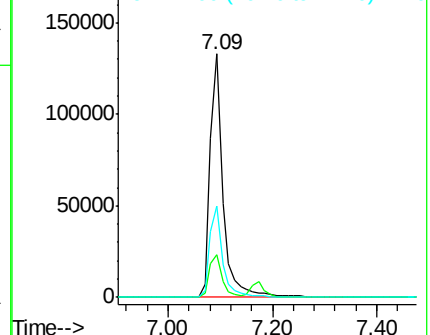

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 10.59 min Scan# 849

Delta R.T. 0.00 min

Lab File: BF077147.D

Acq: 30 Jan 2015 15:15

Tgt Ion: 136 Resp: 112139


Ion Ratio Lower Upper

136 100

137 11.1 8.1 12.1

54 8.4 7.0 10.4

68 4.3 3.7 5.5


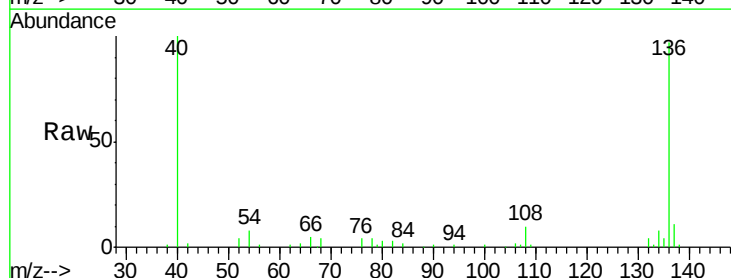



Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0


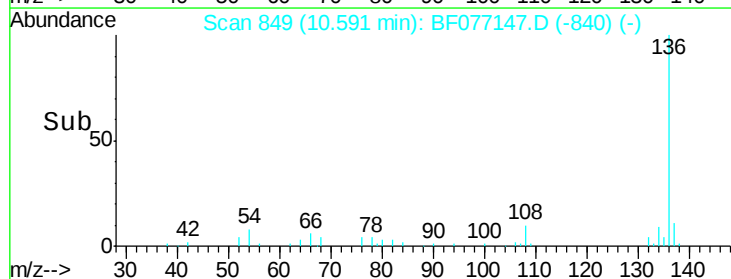
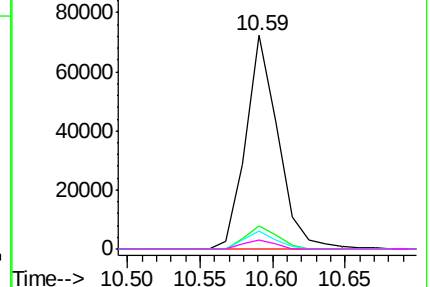


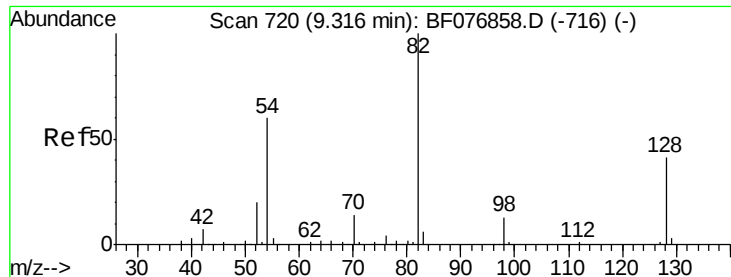

#23
 Nitrobenzene-d5
 Concen: 69.10 ng
 RT: 8.99 min Scan# 709
 Delta R.T. 0.00 min
 Lab File: BF077147.D
 Acq: 30 Jan 2015 15:15




Instrument :
 BNA_F
 ClientSampled :
 PB81569BL

Tgt Ion: 82 Resp: 139859
 Ion Ratio Lower Upper
 82 100
 128 42.4 33.1 49.7
 54 52.7 48.3 72.5

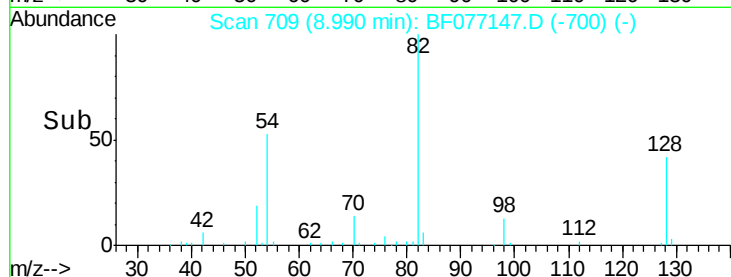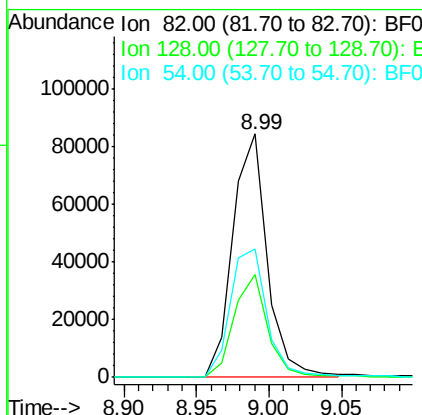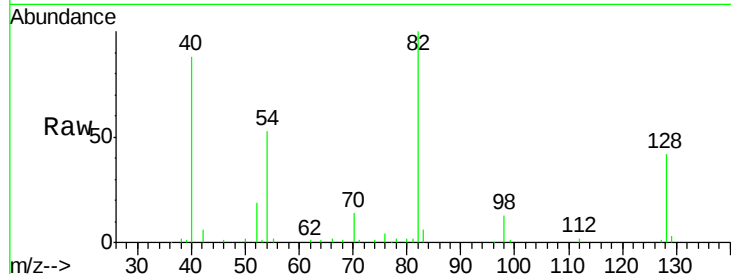

#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 14.72 min Scan# 1210
 Delta R.T. 0.00 min
 Lab File: BF077147.D
 Acq: 30 Jan 2015 15:15

Tgt Ion: 164 Resp: 59802
 Ion Ratio Lower Upper
 164 100
 162 98.6 82.4 123.6
 160 43.7 34.8 52.2

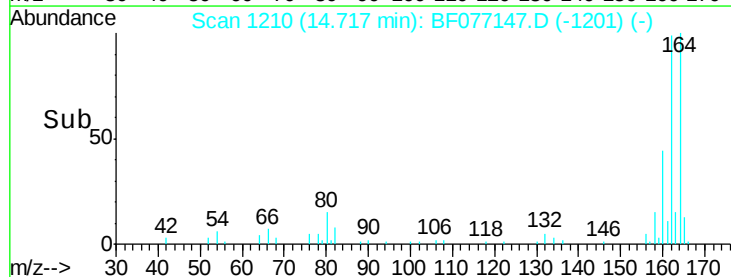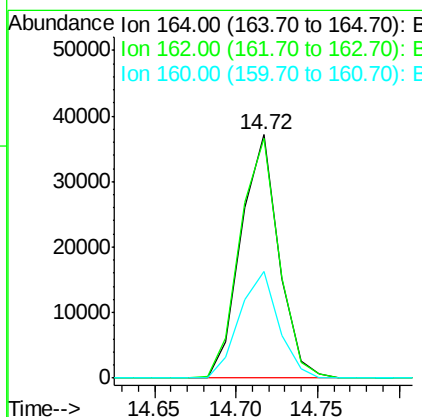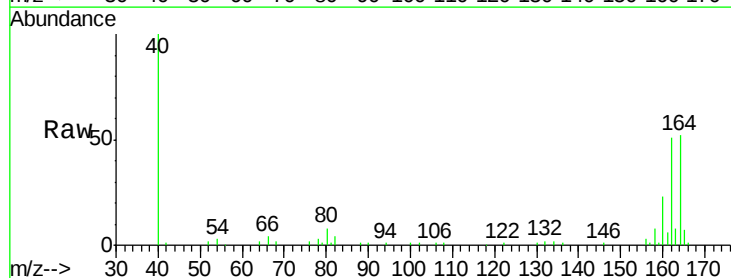



#41

2,4,6-Tribromophenol

Concen: 108.73 ng

RT: 16.45 min Scan# 1362

Delta R.T. 0.00 min

Lab File: BF077147.D

Acq: 30 Jan 2015 15:15

Instrument :

BNA_F

ClientSampleId :

PB81569BL


Tgt Ion:330 Resp: 52780

Ion Ratio Lower Upper

330 100

332 94.2 77.8 116.6




141 50.1 38.5 57.7

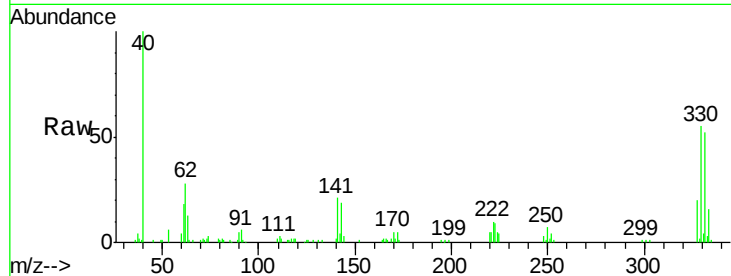

Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

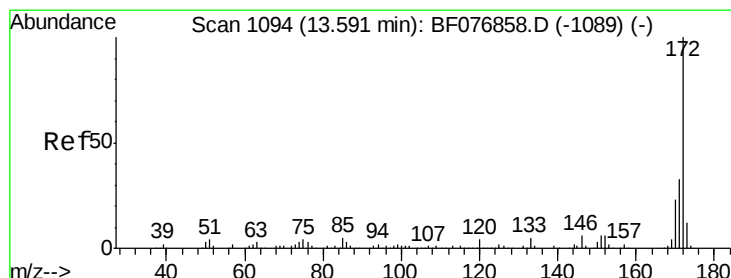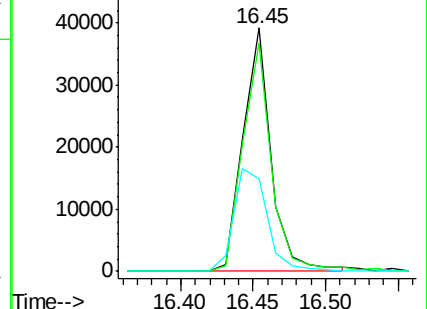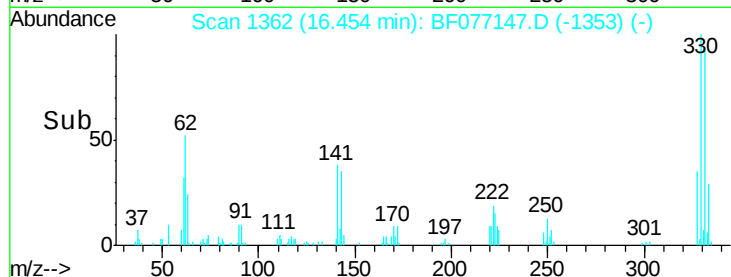

#44

2-Fluorobiphenyl

Concen: 73.87 ng

RT: 13.25 min Scan# 1082

Delta R.T. 0.00 min

Lab File: BF077147.D

Acq: 30 Jan 2015 15:15


Tgt Ion:172 Resp: 290266

Ion Ratio Lower Upper

172 100

171 35.9 26.6 40.0



170 24.3 18.0 27.0

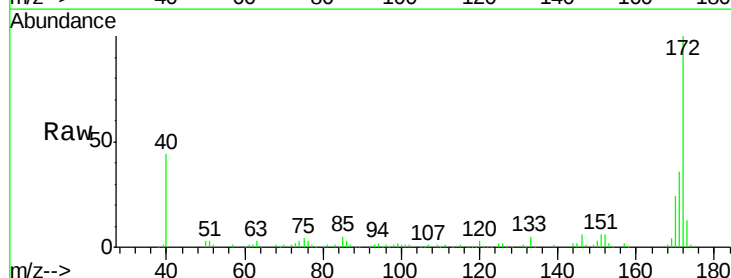


Abundance Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

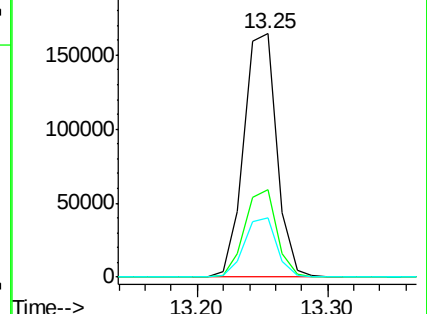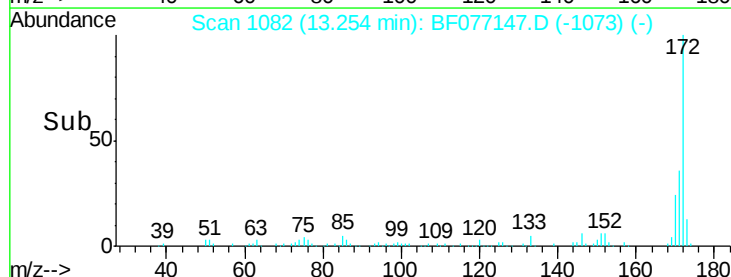


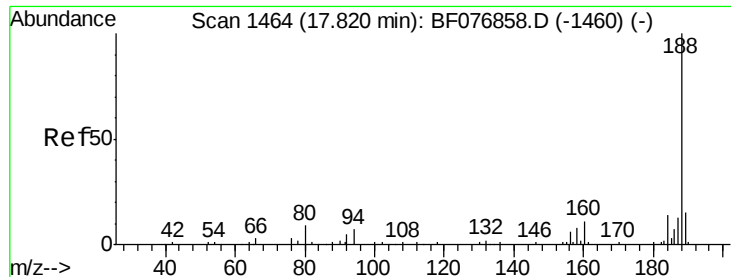



#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 17.57 min Scan# 1460
Delta R.T. 0.00 min
Lab File: BF077147.D
Acq: 30 Jan 2015 15:15

Instrument :
BNA_F
ClientSampled :
PB81569BL

Tgt Ion:188 Resp: 106876
Ion Ratio Lower Upper
188 100
94 7.4 6.0 9.0
80 7.5 6.9 10.3

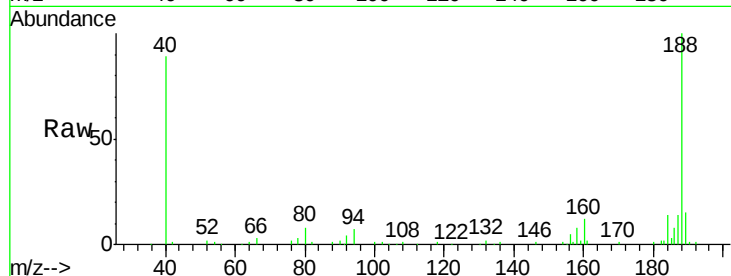


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF0
Ion 80.00 (79.70 to 80.70): BF0

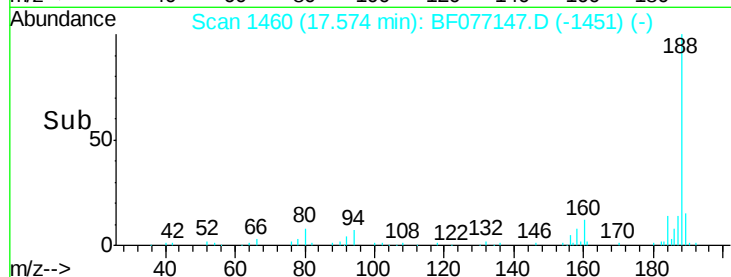
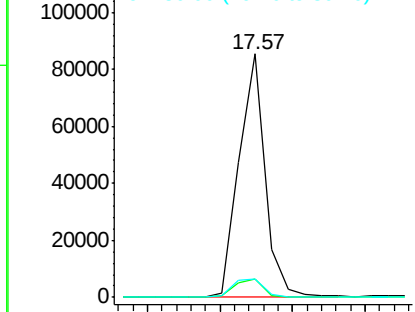


#75
Chrysene-d12
Concen: 20.00 ng
RT: 21.17 min Scan# 1775
Delta R.T. 0.00 min
Lab File: BF077147.D
Acq: 30 Jan 2015 15:15

Tgt Ion:240 Resp: 112786
Ion Ratio Lower Upper
240 100
120 8.5 10.4 15.6#
236 25.7 20.2 30.2

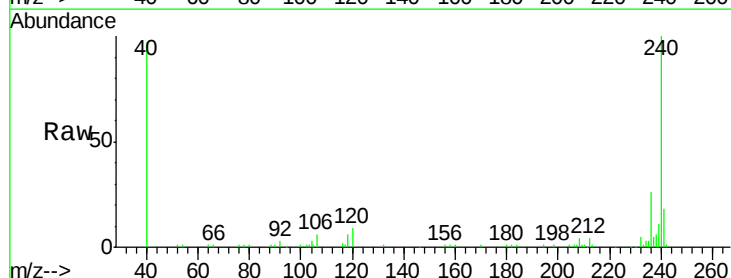

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

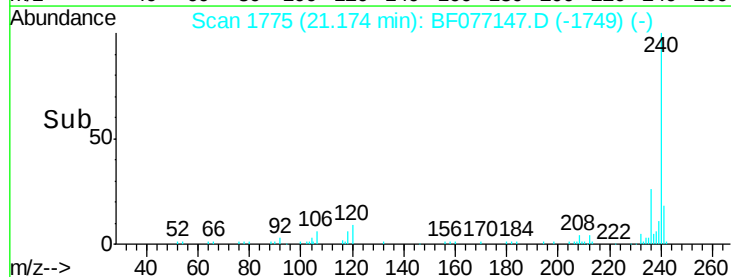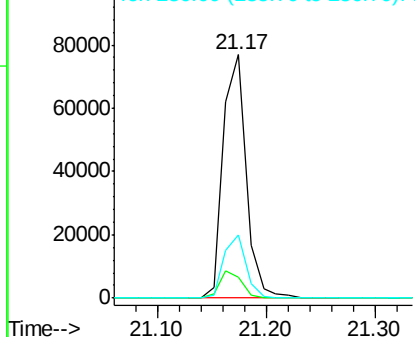



#78

Terphenyl-d14

Concen: 68.90 ng

RT: 19.83 min Scan# 1657

Delta R.T. 0.01 min

Lab File: BF077147.D

Acq: 30 Jan 2015 15:15

Instrument :

BNA_F

ClientSampleId :

PB81569BL


Tgt Ion:244 Resp: 337543

Ion Ratio Lower Upper

244 100

212 7.5 6.3 9.5




122 13.6 10.1 15.1

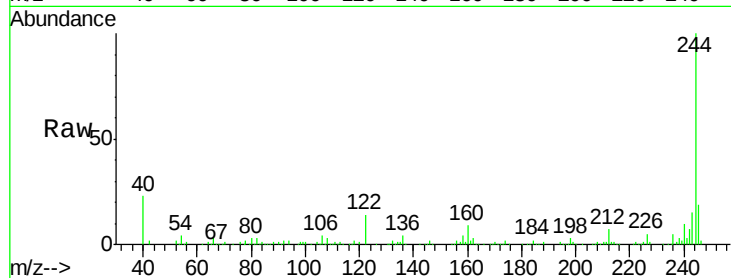

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

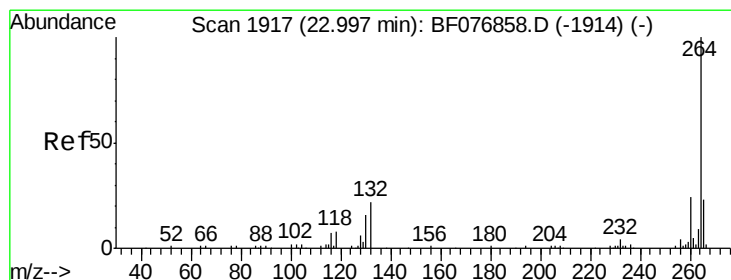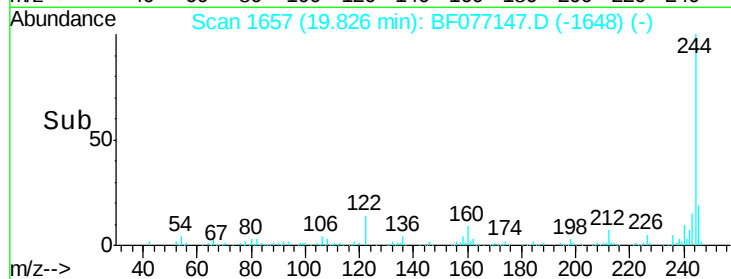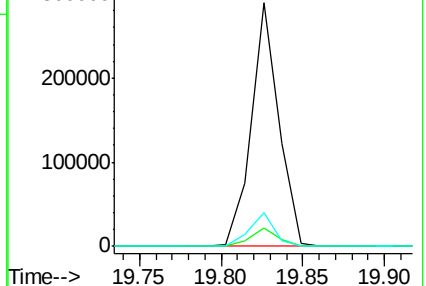

#86

Perylene-d12

Concen: 20.00 ng

RT: 23.17 min Scan# 1950

Delta R.T. 0.00 min

Lab File: BF077147.D

Acq: 30 Jan 2015 15:15


Tgt Ion:264 Resp: 100612

Ion Ratio Lower Upper

264 100

260 23.2 19.0 28.4

265 21.0 18.1 27.1

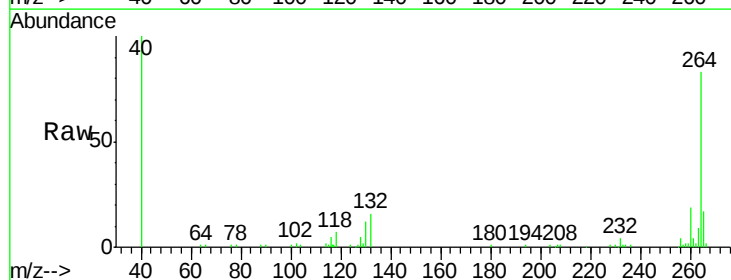

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

