


Data Path : Z:\HPCHEM1\BNA\_F\DATA\BF013015\  
 Data File : BF077145.D  
 Acq On : 30 Jan 2015 10:07  
 Operator : TP/IZ  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA\_F\METHODS\8270-BF011415.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Fri Jan 30 22:48:24 2015

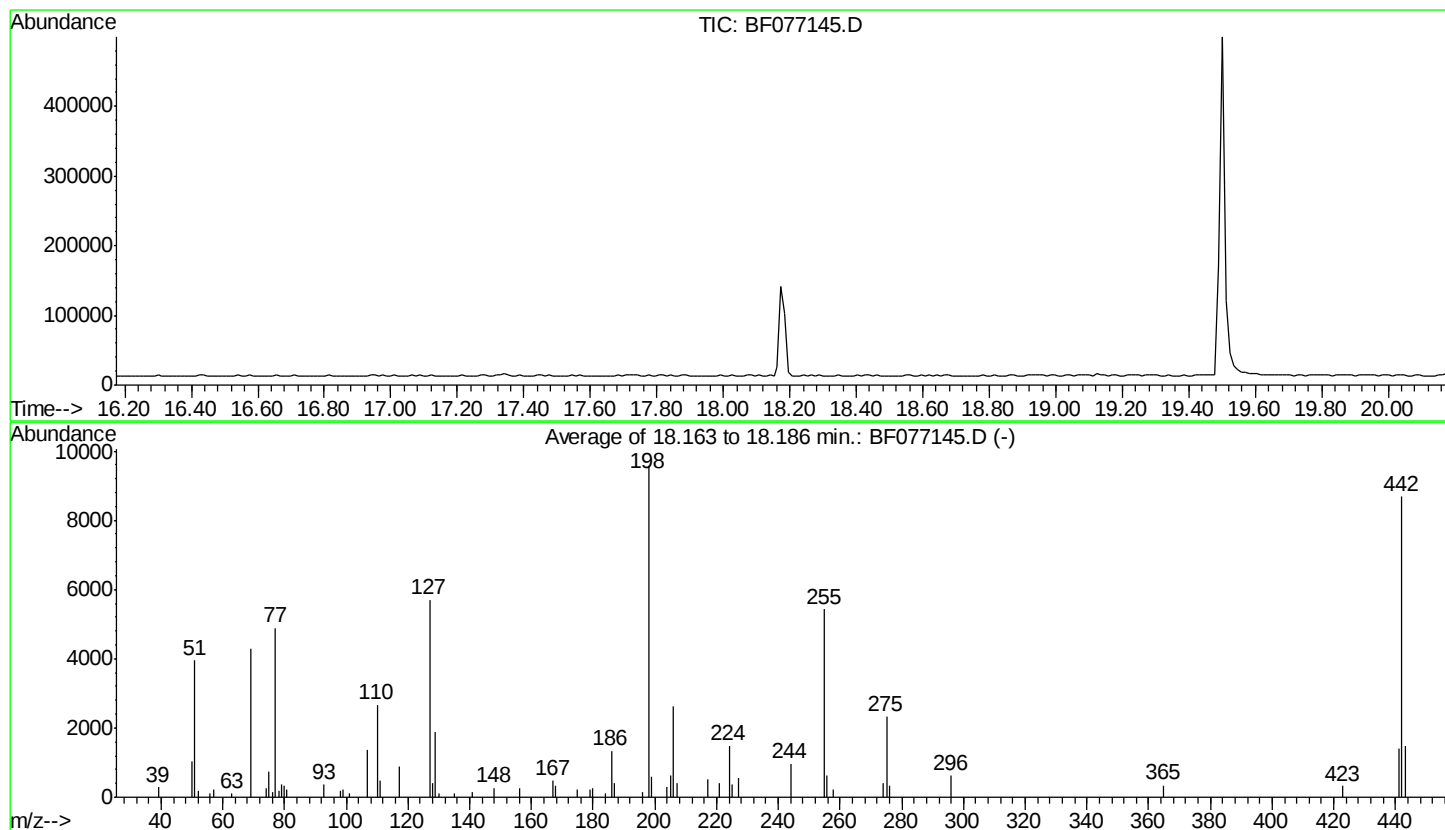

AutoFind: Scans 1494, 1495, 1496; Background Corrected with Scan 1491

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 41.2      | 3942    | PASS             |
| 68          | 69           | 0.00         | 2            | 0.0       | 0       | PASS             |
| 69          | 198          | 0.00         | 100          | 44.9      | 4304    | PASS             |
| 70          | 69           | 0.00         | 2            | 0.0       | 0       | PASS             |
| 127         | 198          | 10           | 80           | 59.5      | 5703    | PASS             |
| 197         | 198          | 0.00         | 2            | 0.0       | 0       | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 9577    | PASS             |
| 199         | 198          | 5            | 9            | 6.1       | 580     | PASS             |
| 275         | 198          | 10           | 60           | 24.3      | 2329    | PASS             |
| 365         | 198          | 1            | 100          | 3.7       | 351     | PASS             |
| 441         | 442          | 0.01         | 24           | 16.1      | 1400    | PASS             |
| 442         | 198          | 50           | 100          | 90.6      | 8680    | PASS             |
| 443         | 442          | 15           | 24           | 17.2      | 1493    | PASS             |