
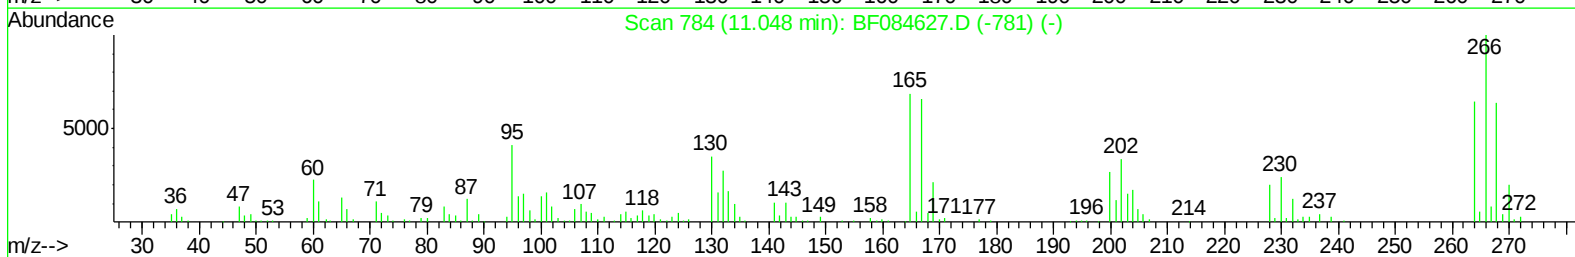
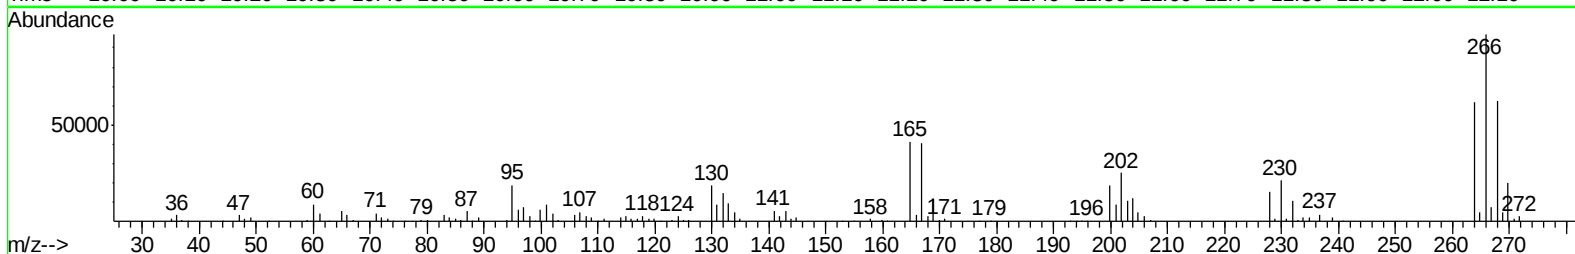


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF013016\
Data File : BF084666.D
Acq On : 30 Jan 2016 6:04
Operator : SJ/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 01 02:30:24 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF012916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 29 12:54:53 2016
Response via : Initial Calibration

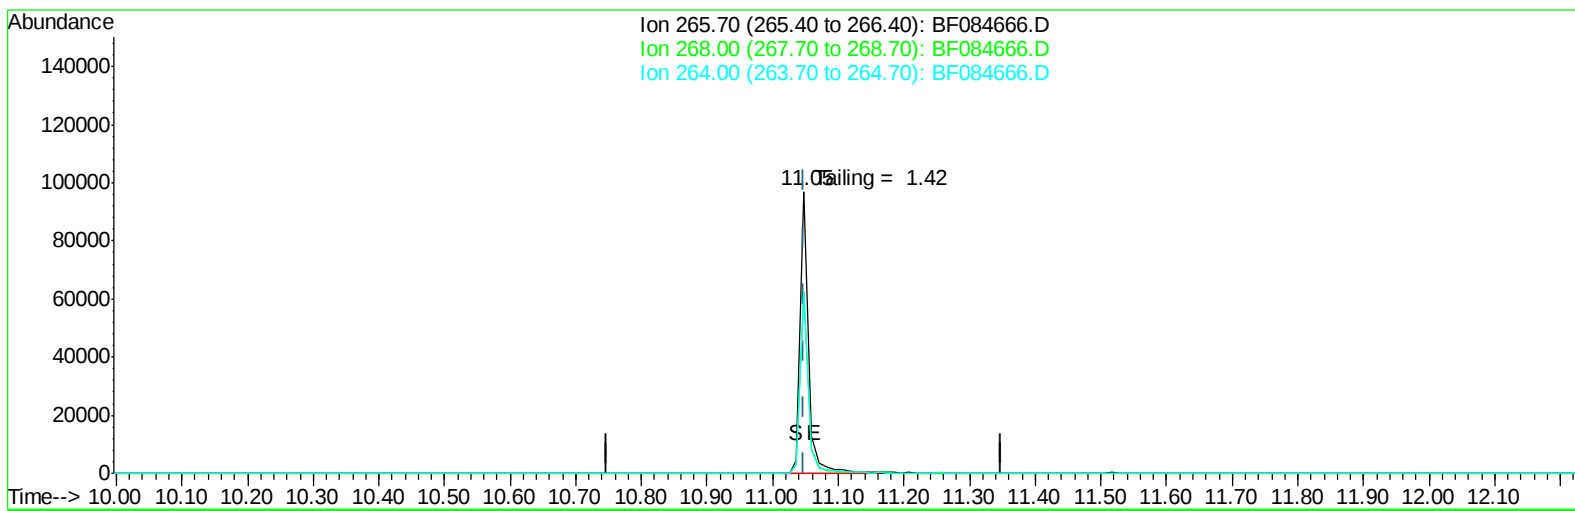

TIC: BF084666.D

(69) Pentachlorophenol (C)




11.048min (-0.000) 0.00ng

response 86979

Ion	Exp%	Act%
265.70	100	100
268.00	65.50	64.66
264.00	62.70	63.94
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF013016\
Data File : BF084666.D
Acq On : 30 Jan 2016 6:04
Operator : SJ/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 01 02:30:24 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF012916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 29 12:54:53 2016
Response via : Initial Calibration

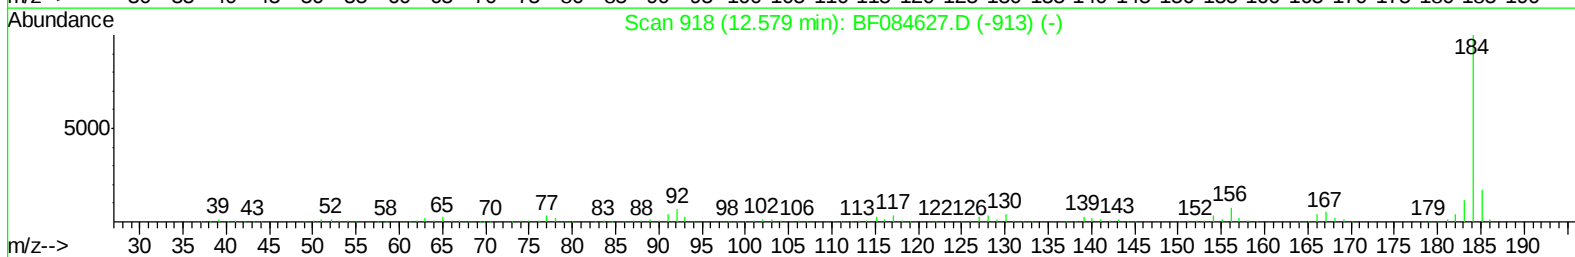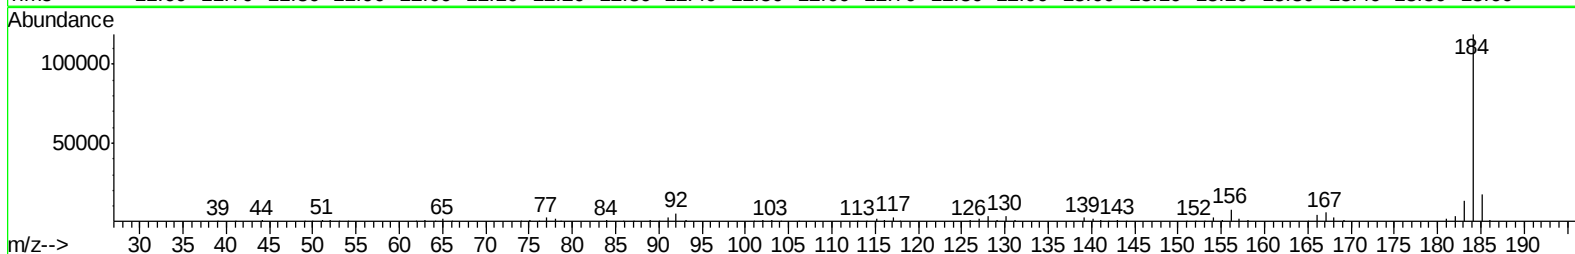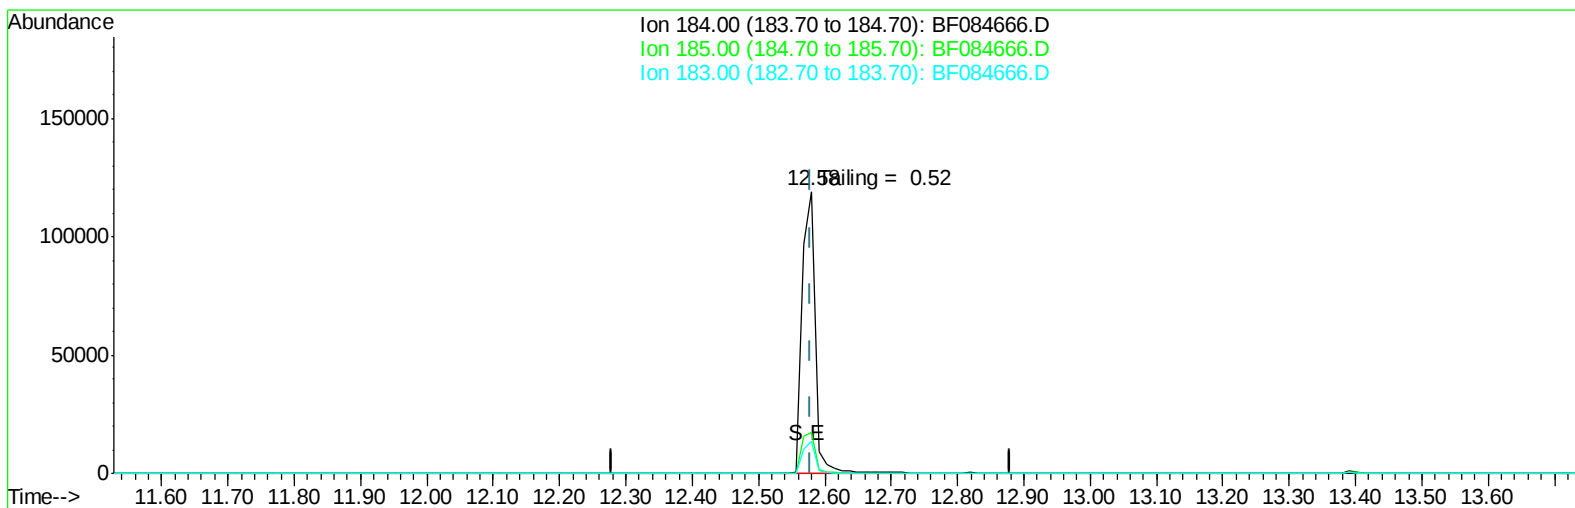

TIC: BF084666.D

(76) Benzidine

12.579min (-0.000) 0.00ng

response 162059

Ion	Exp%	Act%
184.00	100	100
185.00	15.20	14.78
183.00	12.30	11.34
0.00	0.00	0.00