
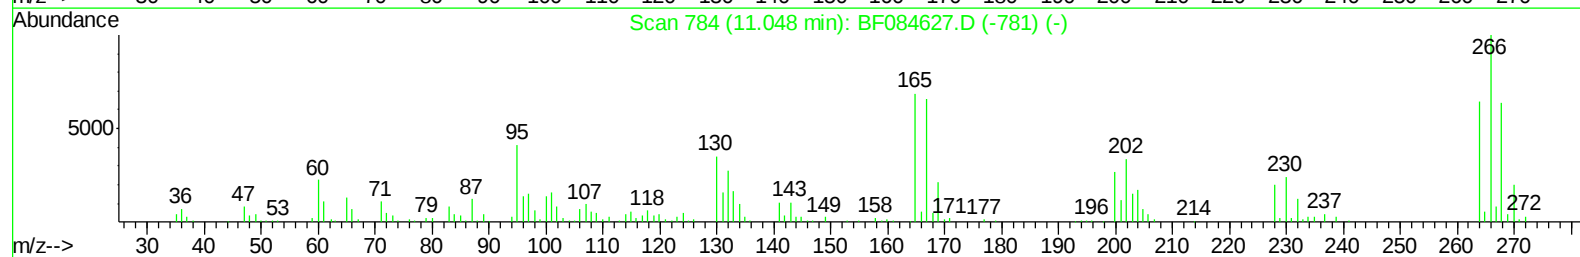
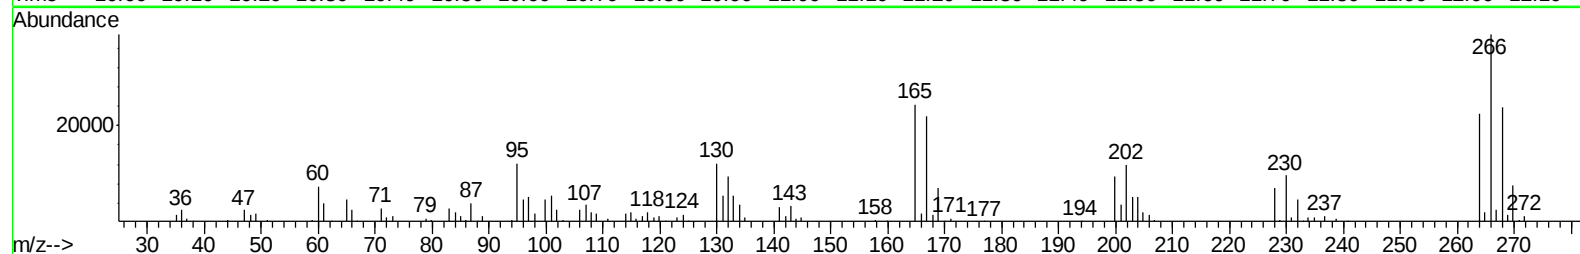


Data Path : Z:\HPCHEM1\BNA\_F\Data\BF013016\  
Data File : BF084693.D  
Acq On : 30 Jan 2016 19:26  
Operator : SJ/IZ  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 01 02:38:26 2016  
Quant Method : Z:\HPCHEM1\BNA\_F\METHODS\8270-BF012916.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Jan 29 12:54:53 2016  
Response via : Initial Calibration

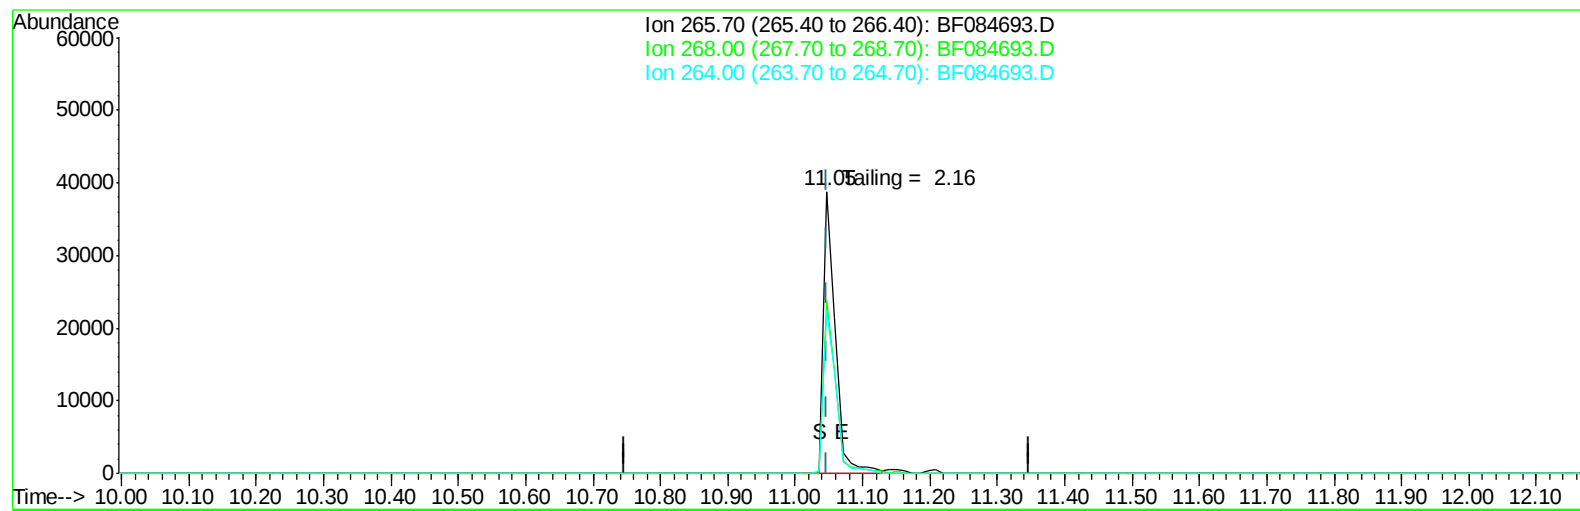

TIC: BF084693.D

(69) Pentachlorophenol (C)




11.048min (-0.000) 16310.82ng

response 47206

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 265.70 | 100   | 100   |
| 268.00 | 65.50 | 61.30 |
| 264.00 | 62.70 | 57.62 |
| 0.00   | 0.00  | 0.00  |

Data Path : Z:\HPCHEM1\BNA\_F\Data\BF013016\  
 Data File : BF084693.D  
 Acq On : 30 Jan 2016 19:26  
 Operator : SJ/IZ  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 01 02:38:26 2016  
 Quant Method : Z:\HPCHEM1\BNA\_F\METHODS\8270-BF012916.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Fri Jan 29 12:54:53 2016  
 Response via : Initial Calibration

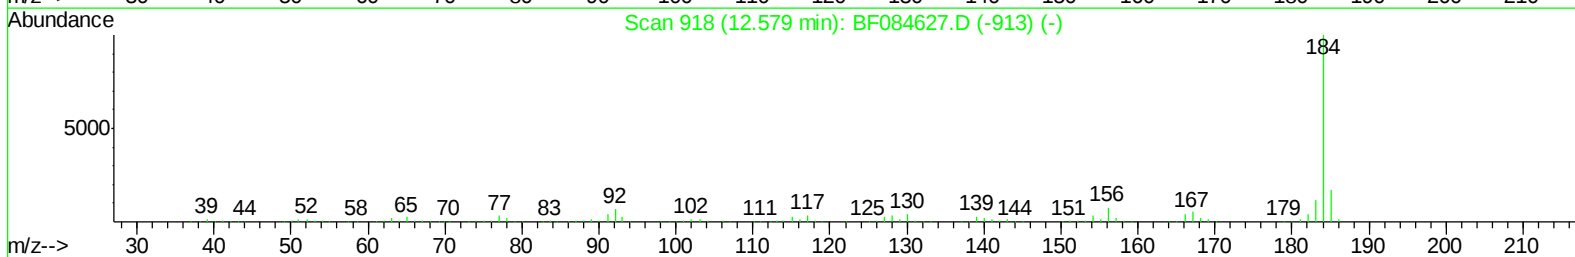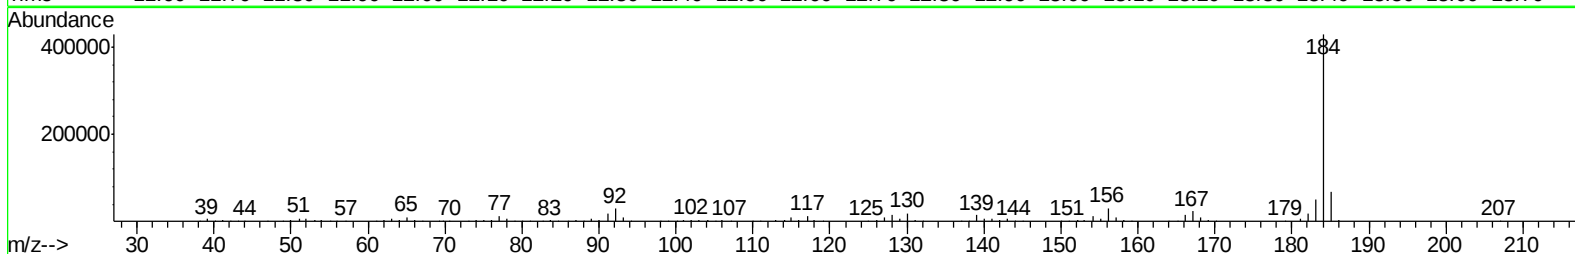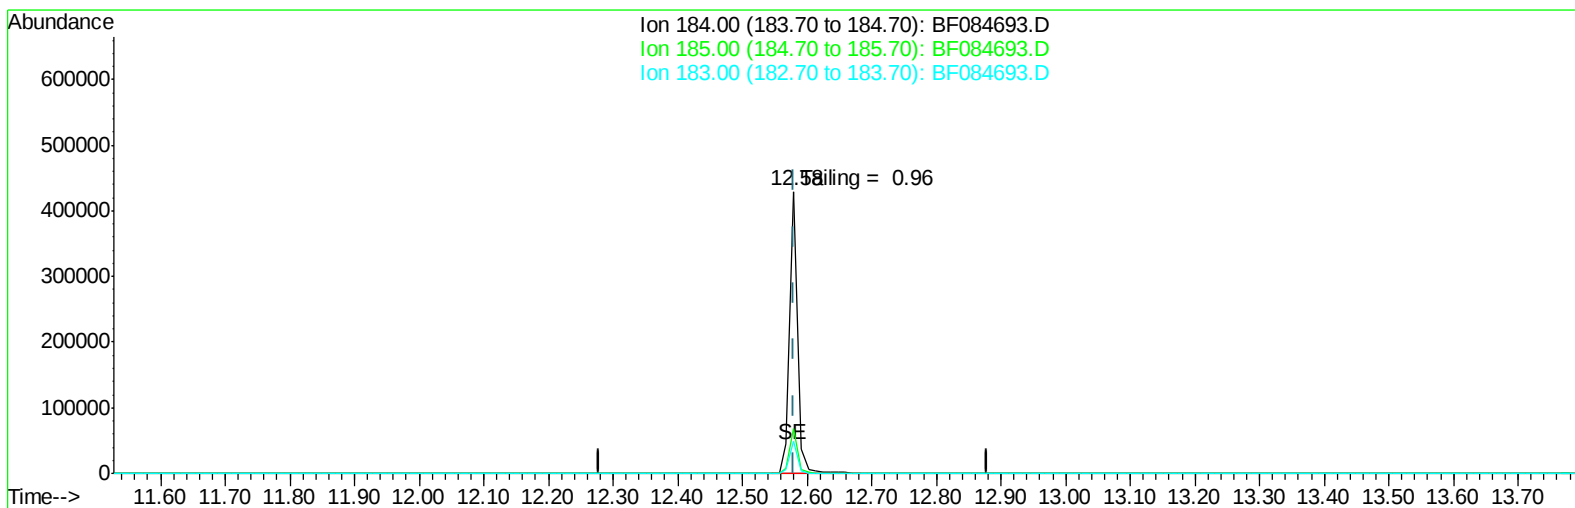

TIC: BF084693.D

(76) Benzidine

12.579min (-0.000) 24649.29ng

response 364680

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 184.00 | 100   | 100   |
| 185.00 | 15.20 | 15.85 |
| 183.00 | 12.30 | 11.54 |
| 0.00   | 0.00  | 0.00  |