


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF013016\
 Data File : BF084666.D
 Acq On : 30 Jan 2016 6:04
 Operator : SJ/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF012916.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jan 29 12:54:53 2016

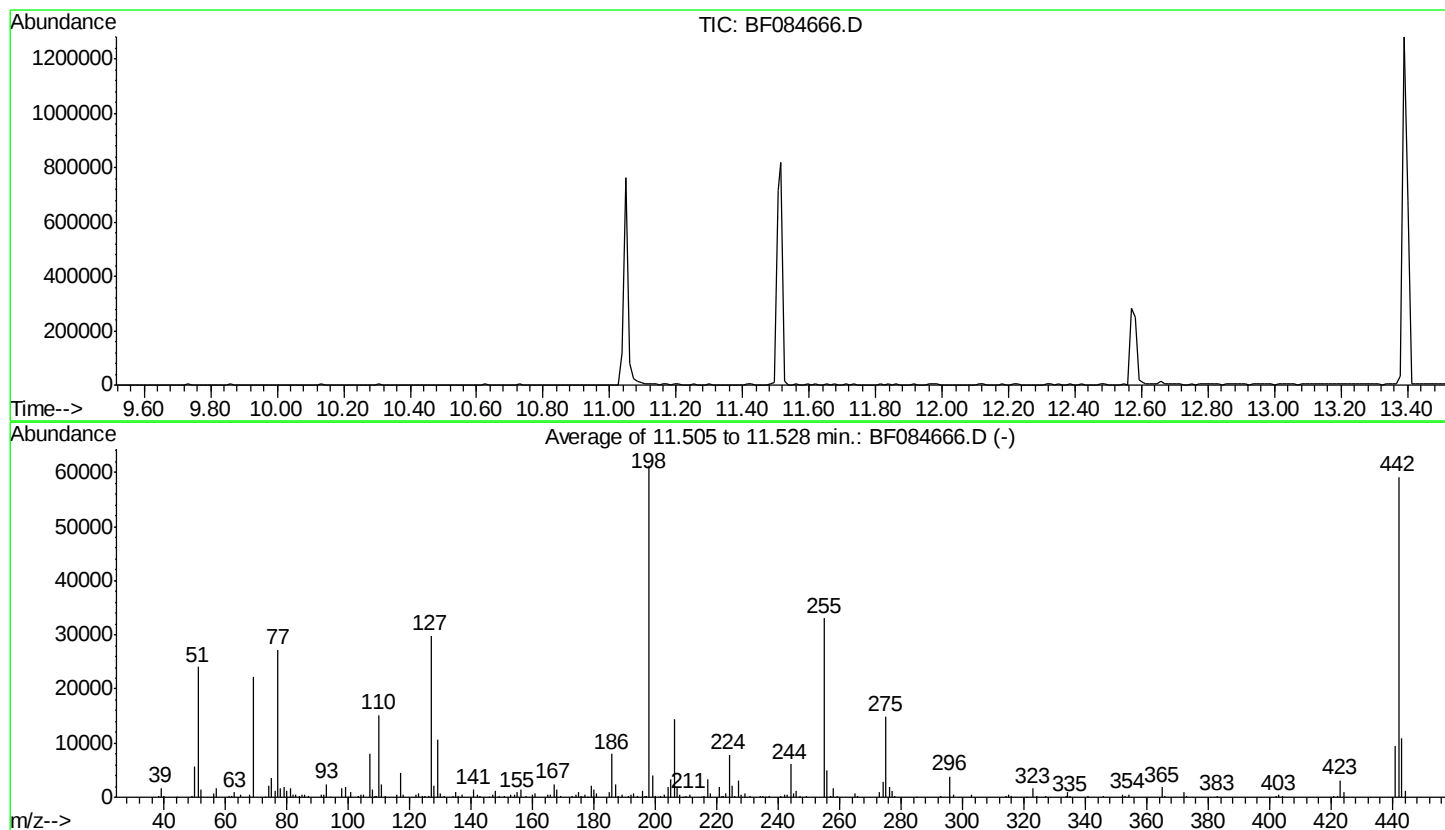

AutoFind: Scans 824, 825, 826; Background Corrected with Scan 820

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.3	24042	PASS
68	69	0.00	2	2.0	436	PASS
69	198	0.00	100	36.3	22205	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	48.8	29904	PASS
197	198	0.00	2	0.3	202	PASS
198	198	100	100	100.0	61252	PASS
199	198	5	9	6.7	4107	PASS
275	198	10	60	24.3	14886	PASS
365	198	1	100	3.0	1818	PASS
441	442	0.01	24	16.0	9484	PASS
442	198	50	100	96.5	59126	PASS
443	442	15	24	18.6	10993	PASS