
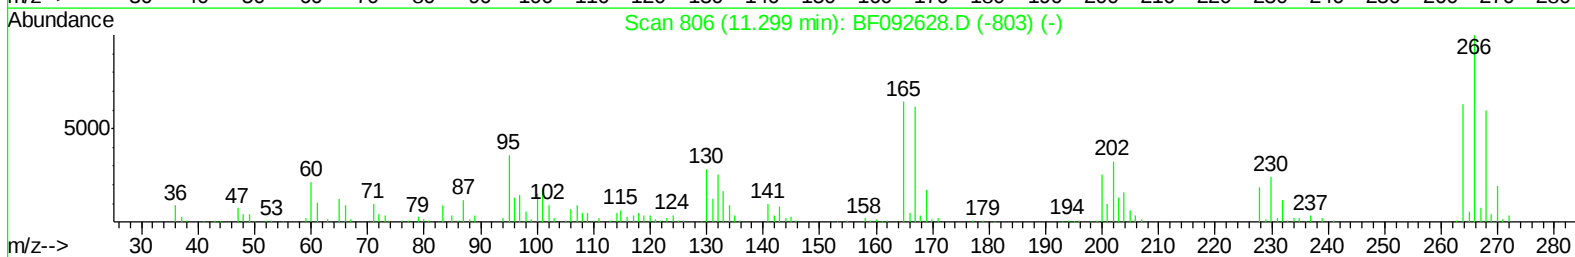
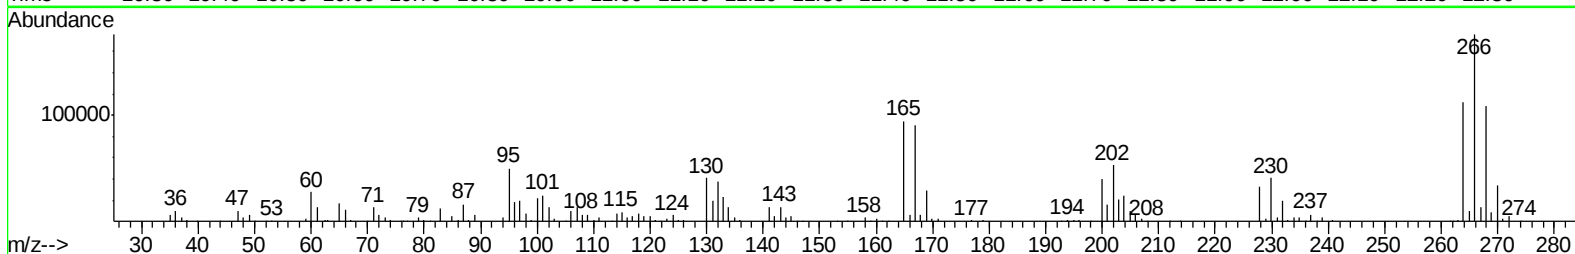


Data Path : Z:\HPCHEM1\BNA_F\Data\BF013017\
Data File : BF092640.D
Acq On : 30 Jan 2017 18:12
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 31 07:58:19 2017
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF013017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 30 14:50:05 2017
Response via : Initial Calibration

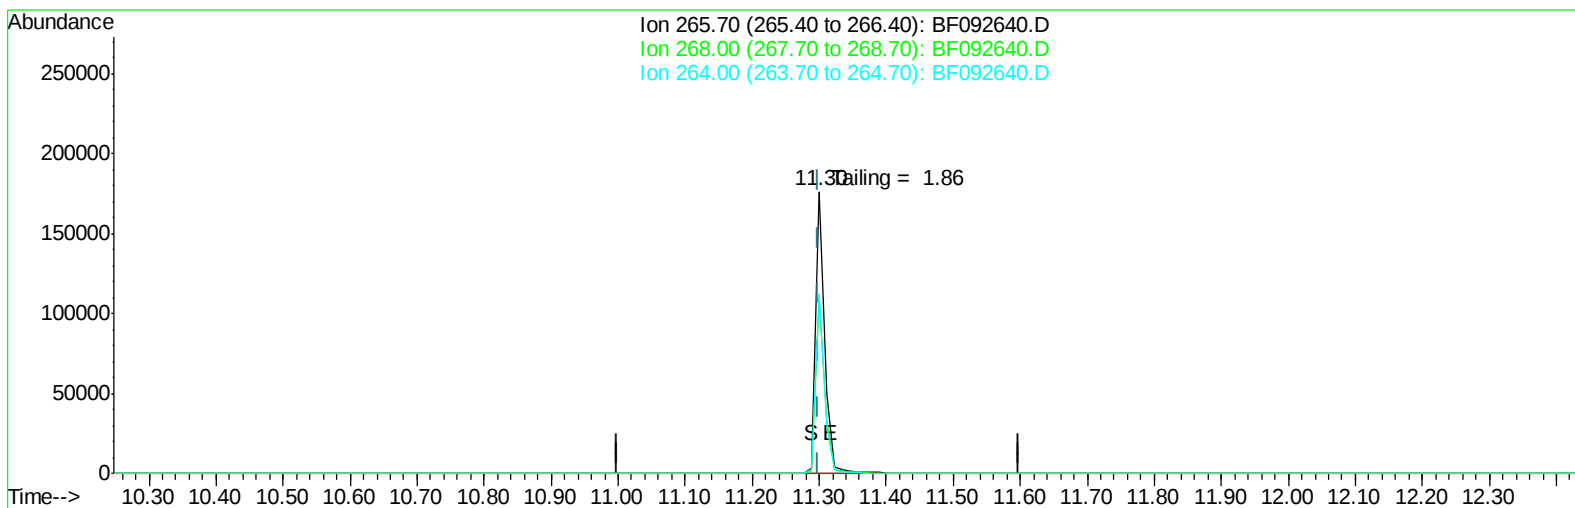

TIC: BF092640.D

(69) Pentachlorophenol (C)




11.299min (+0.000) 0.00ng

response 164757

Ion	Exp%	Act%
265.70	100	100
268.00	66.60	61.74
264.00	62.90	63.78
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\Data\BF013017\
Data File : BF092640.D
Acq On : 30 Jan 2017 18:12
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 31 07:58:19 2017
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF013017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 30 14:50:05 2017
Response via : Initial Calibration

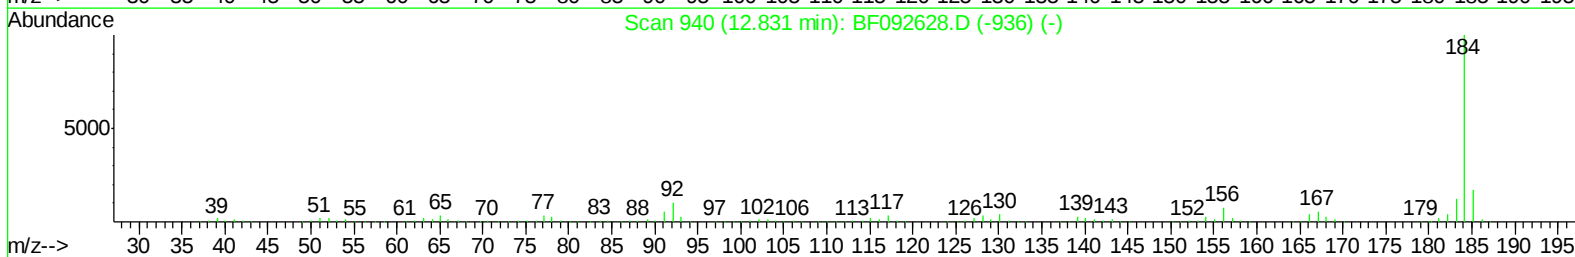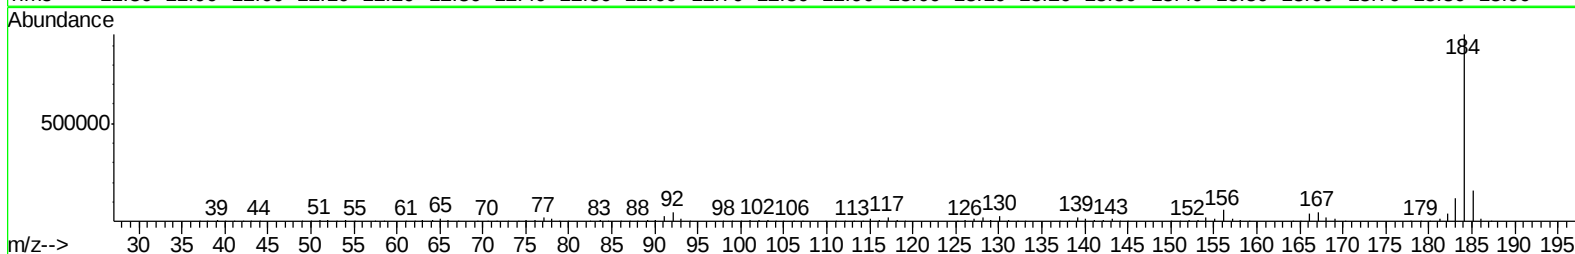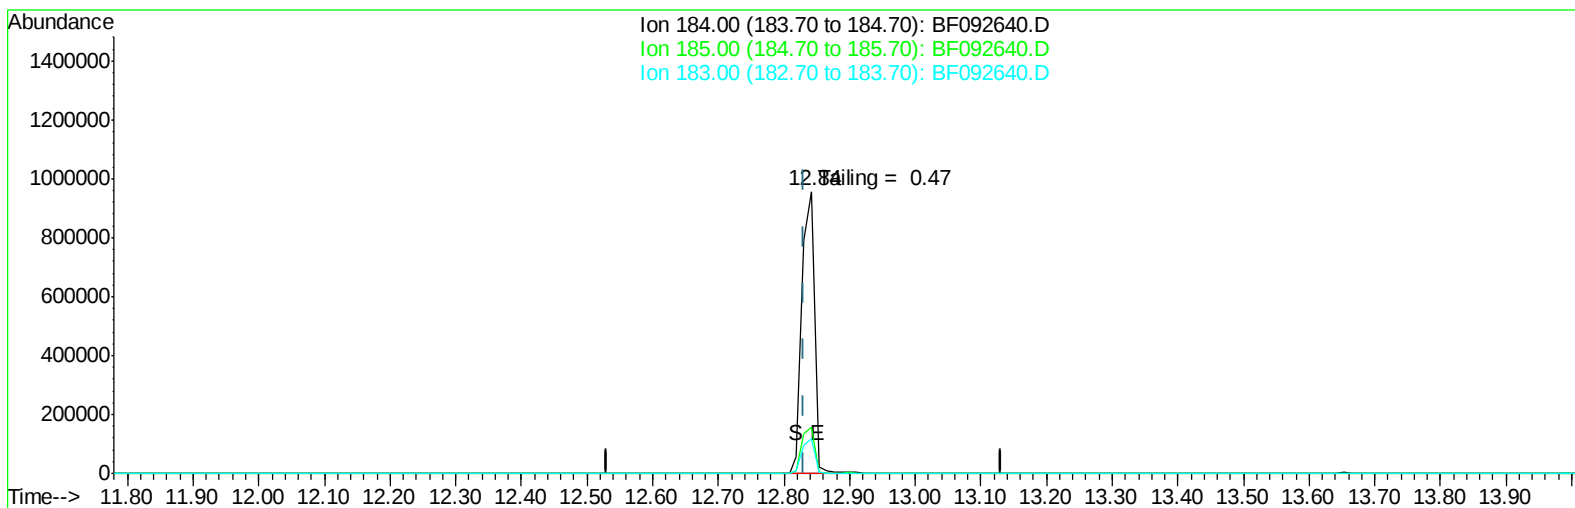

TIC: BF092640.D

(76) Benzidine

12.842min (+0.011) 0.00ng

response 1277308

Ion	Exp%	Act%
184.00	100	100
185.00	16.70	16.26
183.00	11.50	12.07
0.00	0.00	0.00