
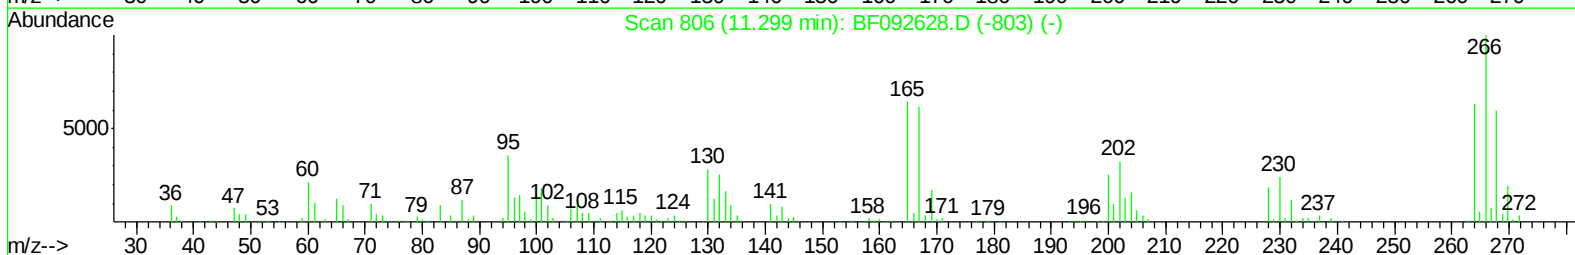
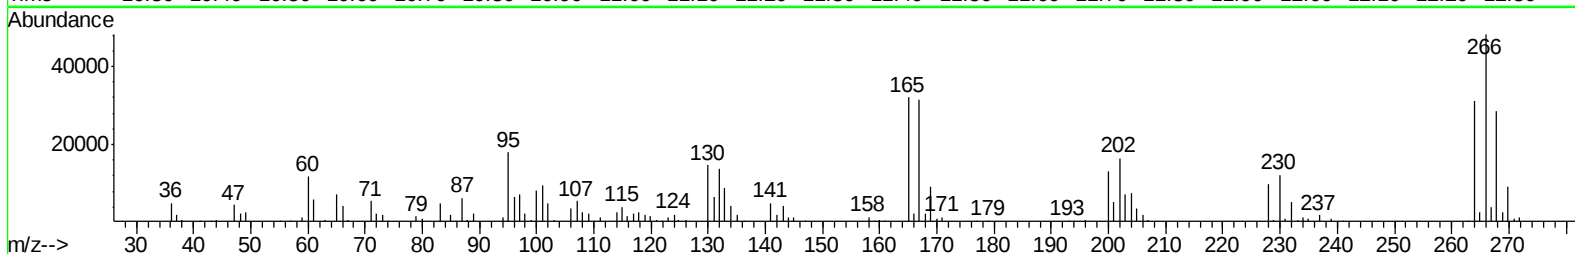


Data Path : Z:\HPCHEM1\BNA_F\Data\BF013017\
Data File : BF092663.D
Acq On : 31 Jan 2017 5:43
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 31 07:59:12 2017
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF013017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 30 14:50:05 2017
Response via : Initial Calibration

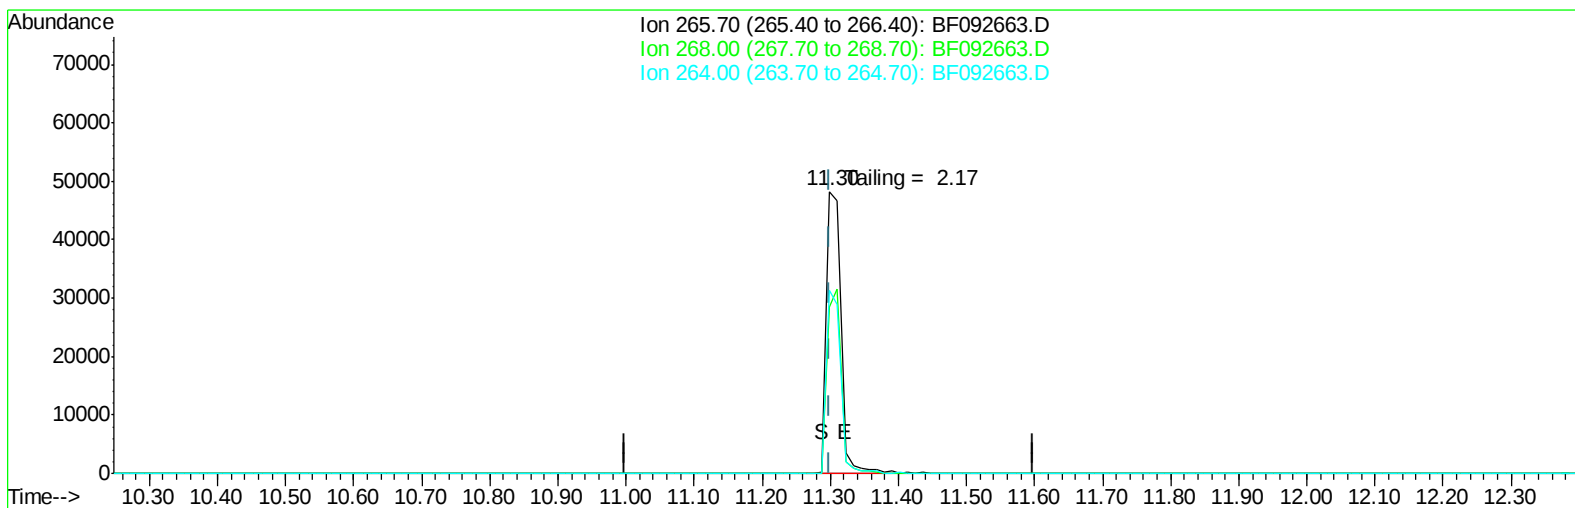

TIC: BF092663.D

(69) Pentachlorophenol (C)




11.299min (+0.000) 0.00ng

response 70502

Ion	Exp%	Act%
265.70	100	100
268.00	66.60	58.92
264.00	62.90	64.96
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\Data\BF013017\
Data File : BF092663.D
Acq On : 31 Jan 2017 5:43
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 31 07:59:12 2017
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF013017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 30 14:50:05 2017
Response via : Initial Calibration

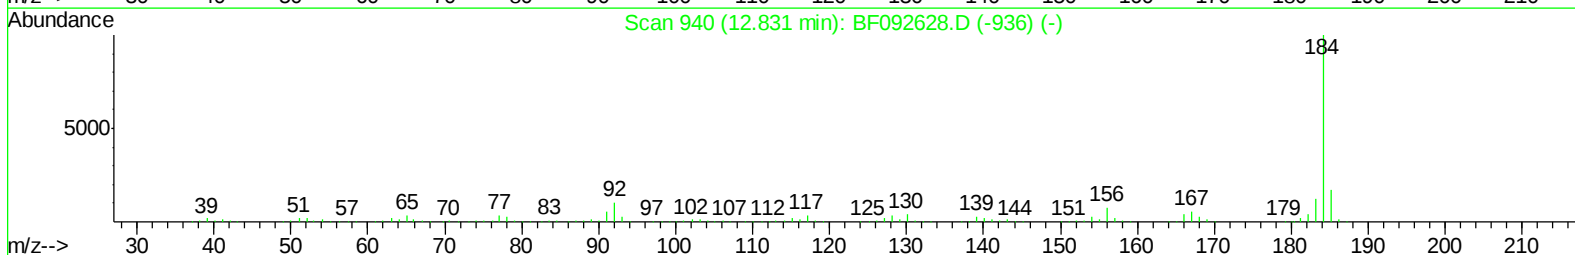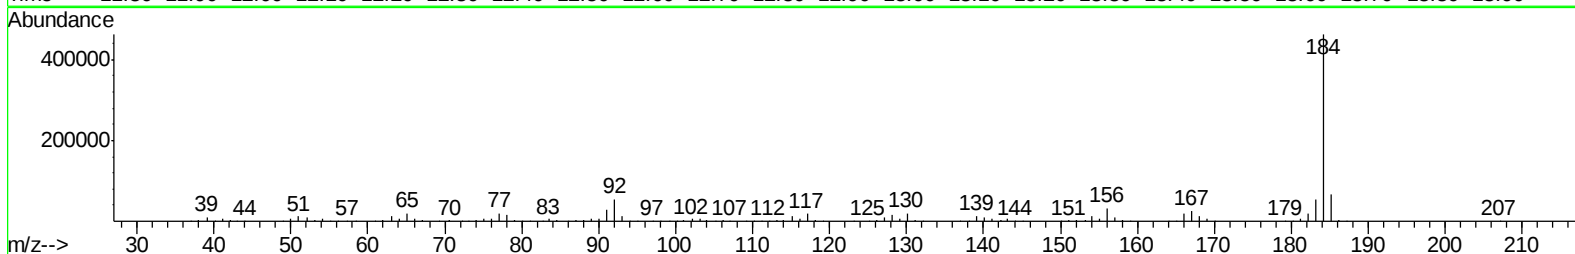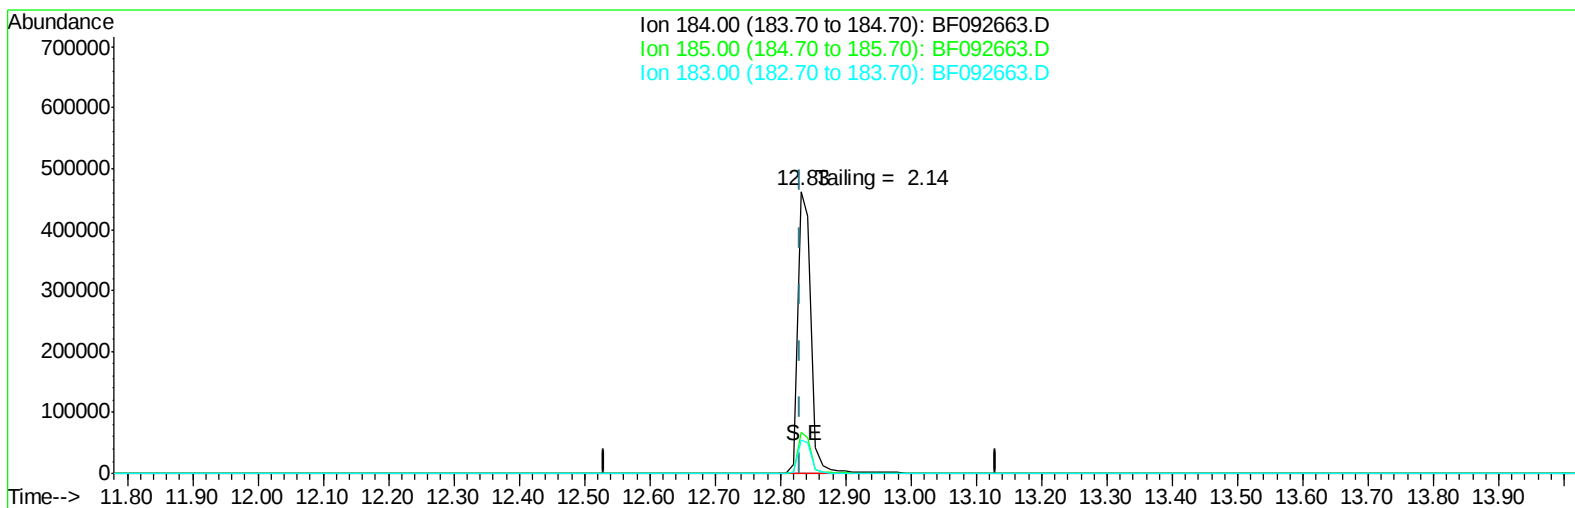

TIC: BF092663.D

(76) Benzidine

12.831min (+0.000) 53863.21ng

response 677101

Ion	Exp%	Act%
184.00	100	100
185.00	16.70	14.70
183.00	11.50	12.02
0.00	0.00	0.00