

Data Path : Z:\HPCHEM1\BNA F\DATA\BF013017\
 Data File : BF092672.D
 Acq On : 31 Jan 2017 9:56
 Operator : SJ/MA
 Sample : I1551-03
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 W-37

Quant Time: Jan 31 10:31:07 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF013017.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jan 30 14:50:05 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.96	152	158702	20.00	ng	-0.01
21) Naphthalene-d8	8.26	136	618747	20.00	ng	0.00
38) Acenaphthene-d10	10.01	164	269629	20.00	ng	0.00
63) Phenanthrene-d10	11.49	188	372224	20.00	ng	0.00
75) Chrysene-d12	14.13	240	310154	20.00	ng	-0.01
86) Perylene-d12	15.61	264	211427	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.57	112	650552	70.33	ng	0.00
7) Phenol-d6	6.60	99	526176	44.21	ng	0.00
23) Nitrobenzene-d5	7.53	82	902018	81.18	ng	-0.01
41) 2,4,6-Tribromophenol	10.81	330	243165	124.69	ng	0.00
44) 2-Fluorobiphenyl	9.33	172	1553246	104.36	ng	0.00
78) Terphenyl-d14	13.08	244	1049562	79.51	ng	0.00


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF013017\
Data File : BF092672.D
Acq On : 31 Jan 2017 9:56
Operator : SJ/MA
Sample : I1551-03
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
W-37

Quant Time: Jan 31 10:31:07 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF013017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 30 14:50:05 2017
Response via : Initial Calibration

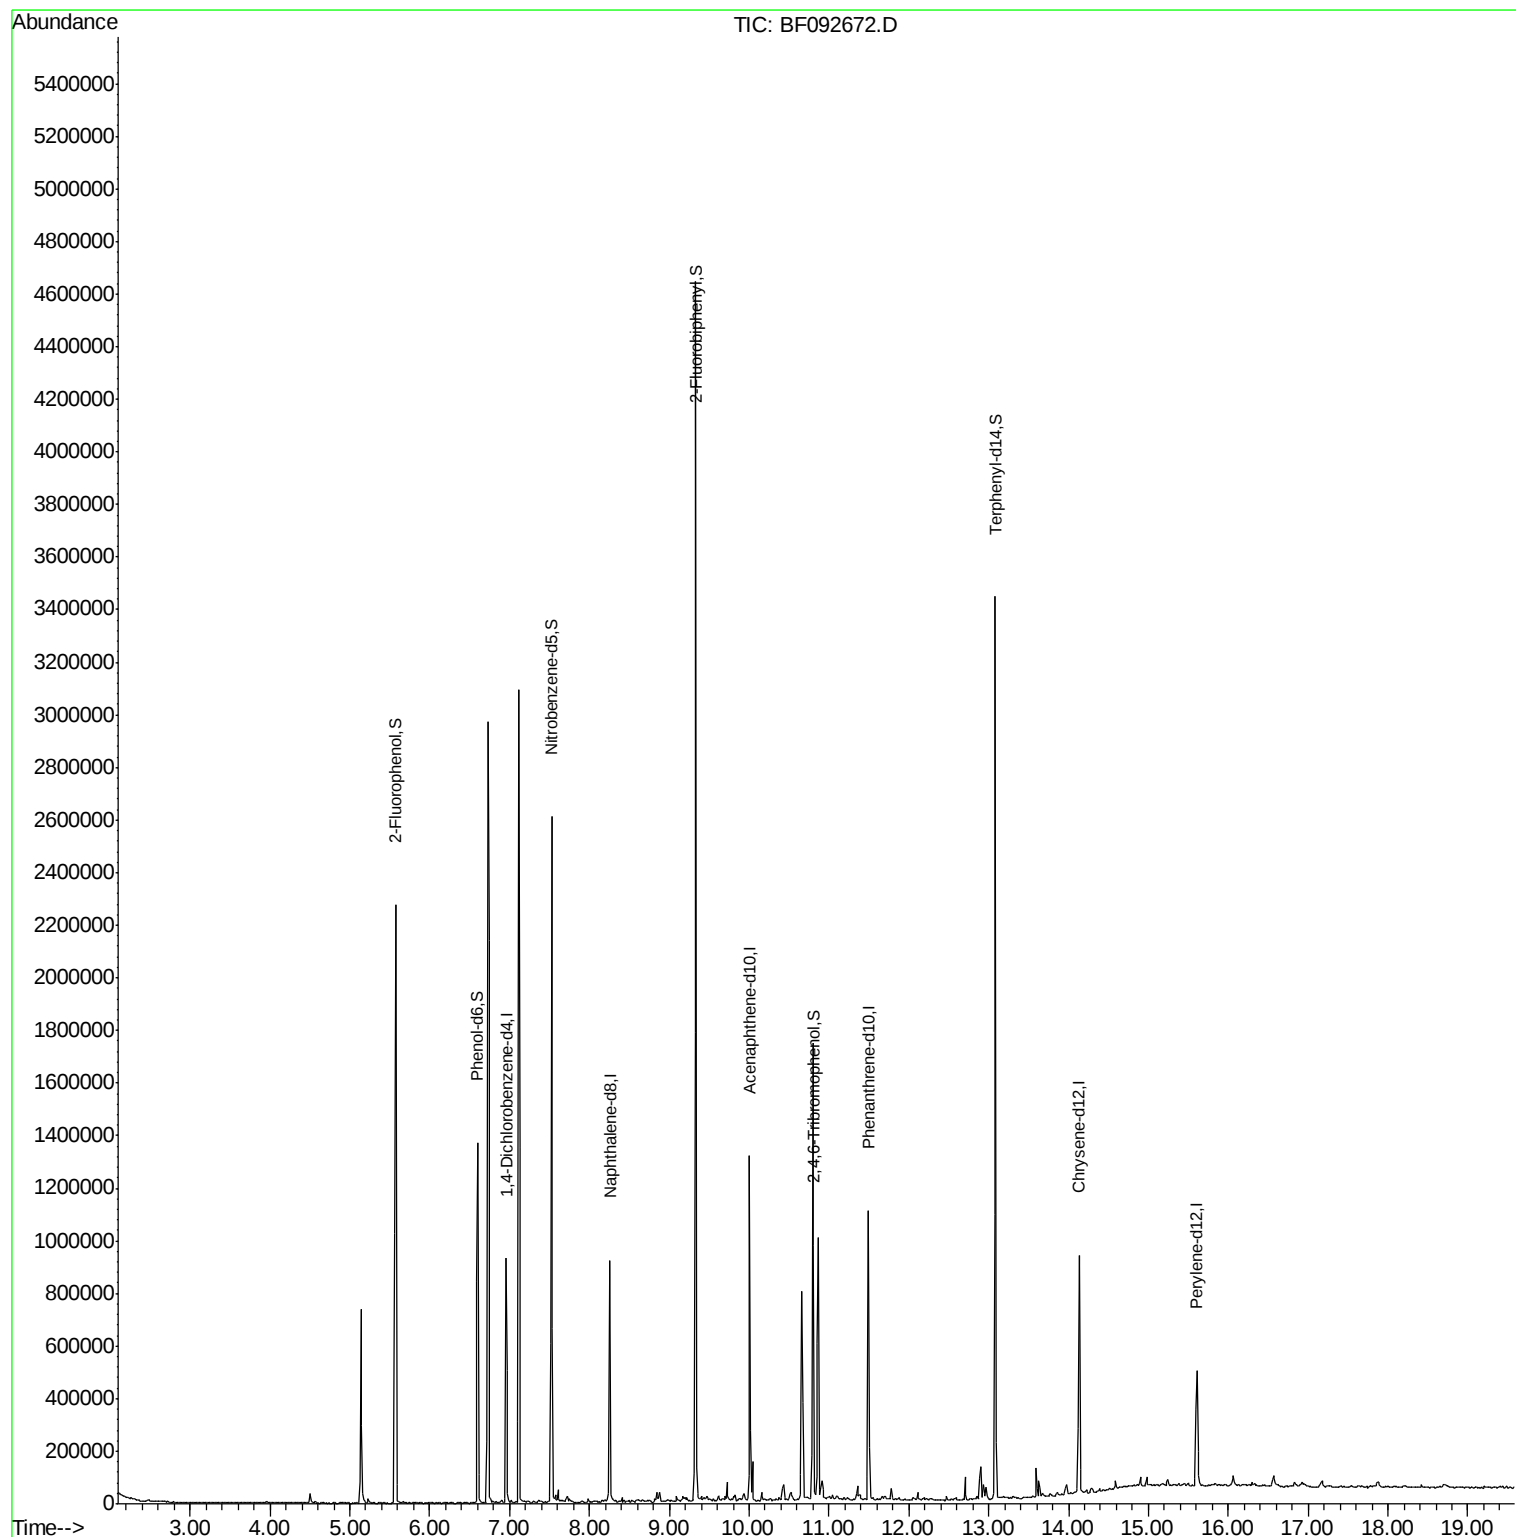

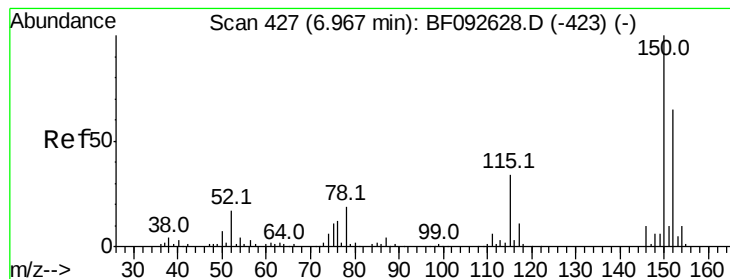

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 6.96 min Scan# 426

Delta R.T. -0.01 min

Lab File: BF092672.D

Acq: 31 Jan 2017 9:56

Instrument :

BNA_F

ClientSampled :

W-37


Tot Ion:152 Resp: 158702

Ion Ratio Lower Upper

152 100

150 160.0 124.9 187.3




115 70.3 46.0 69.0#

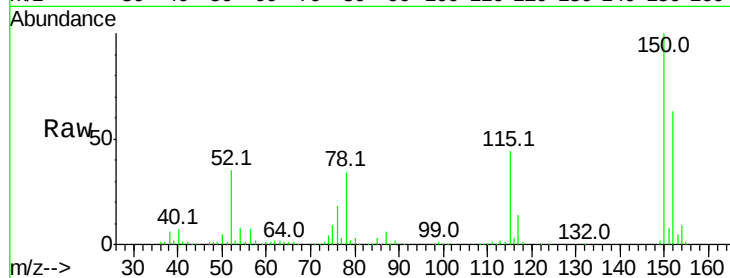

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

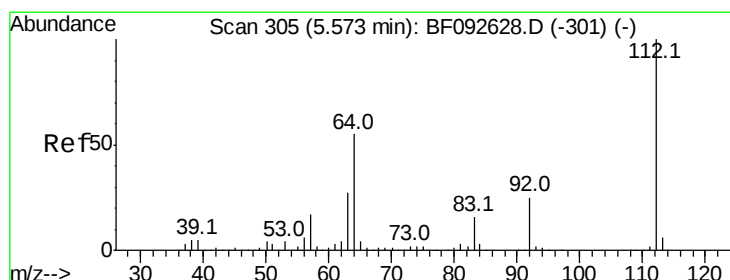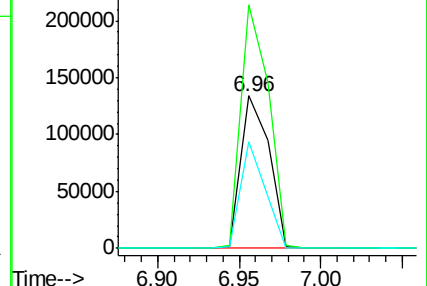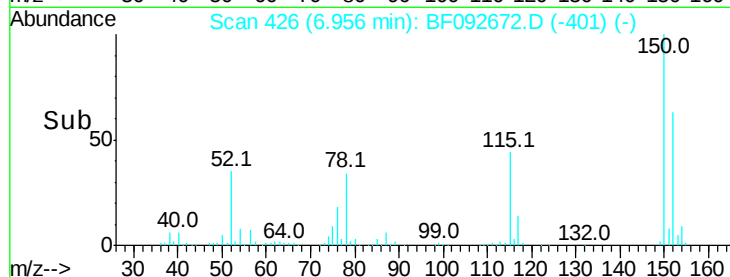

#5

2-Fluorophenol

Concen: 70.33 ng

RT: 5.57 min Scan# 305

Delta R.T. 0.00 min

Lab File: BF092672.D

Acq: 31 Jan 2017 9:56


Tgt Ion:112 Resp: 650552

Ion Ratio Lower Upper

112 100

64 60.1 46.1 69.1



63 30.4 23.8 35.6

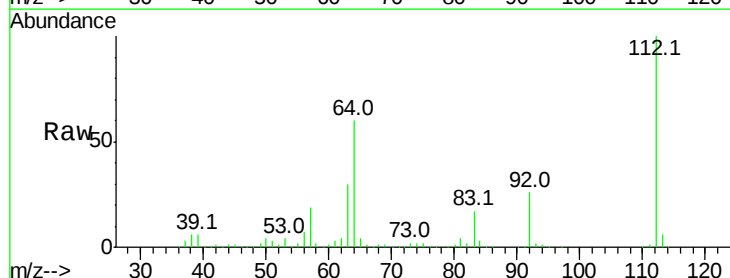


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0

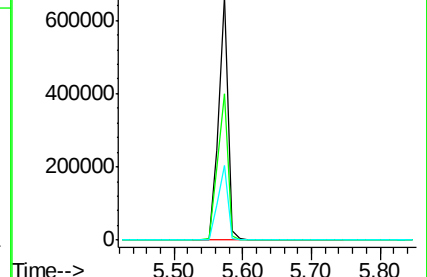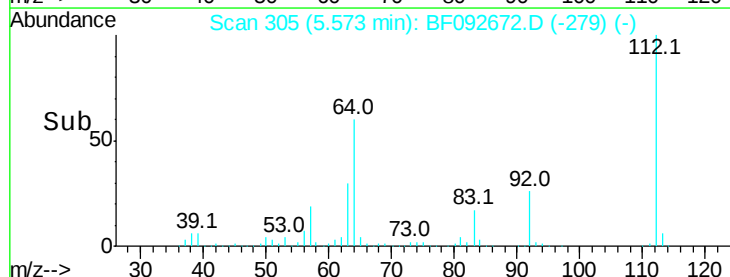

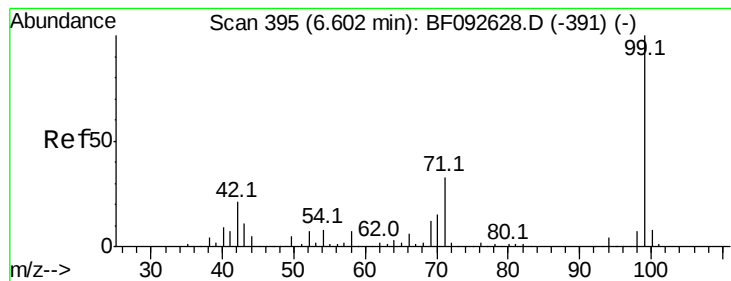

#7

Phenol-d6

Concen: 44.21 ng

RT: 6.60 min Scan# 395

Delta R.T. -0.00 min

Lab File: BF092672.D

Acq: 31 Jan 2017 9:56

Instrument :

BNA_F

ClientSampleId :

W-37


Tot Ion: 99 Resp: 526176

Ion Ratio Lower Upper

99 100

42 17.5 15.6 23.4




71 30.5 27.5 41.3

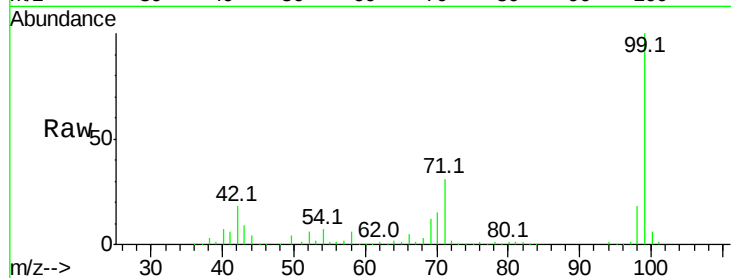

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

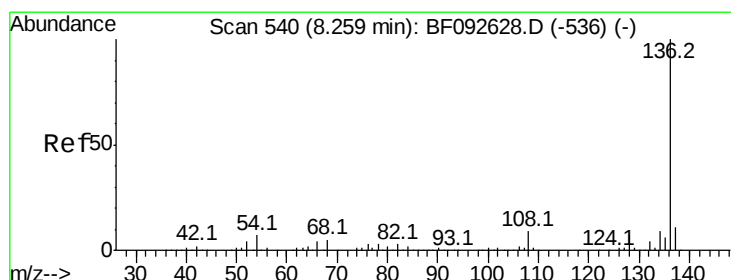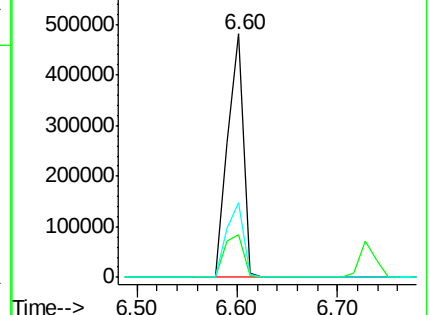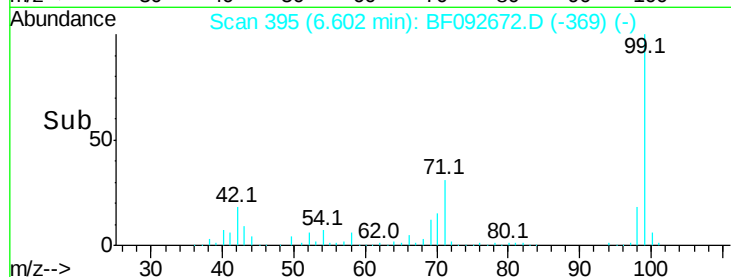

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 8.26 min Scan# 540

Delta R.T. -0.00 min

Lab File: BF092672.D

Acq: 31 Jan 2017 9:56

Tgt Ion: 136 Resp: 618747


Ion Ratio Lower Upper

136 100

137 10.2 8.4 12.6

54 6.7 4.5 6.7

68 4.9 3.6 5.4


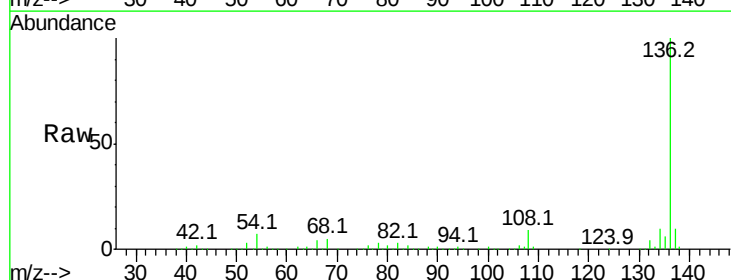



Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0

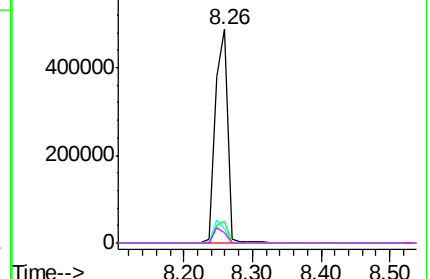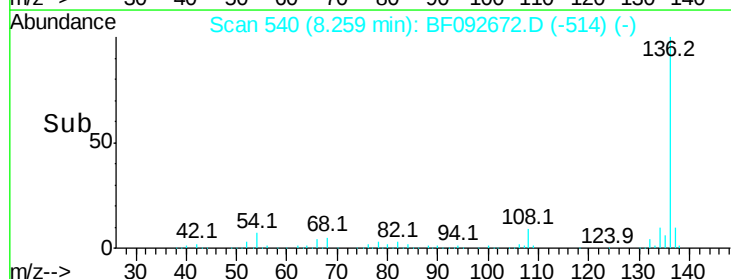


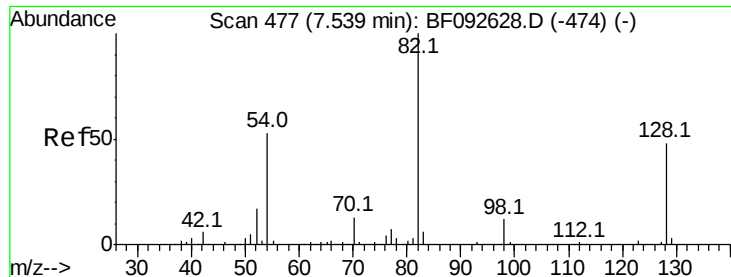




#23
Nitrobenzene-d5
Concen: 81.18 ng
RT: 7.53 min Scan# 476
Delta R.T. -0.01 min
Lab File: BF092672.D
Acq: 31 Jan 2017 9:56

Instrument :
BNA_F
ClientSampled :
W-37

Tot Ion	82	Resp	902018
Ion Ratio	100	Lower	Upper
128	39.8	34.6	52.0
54	60.1	39.5	59.3#

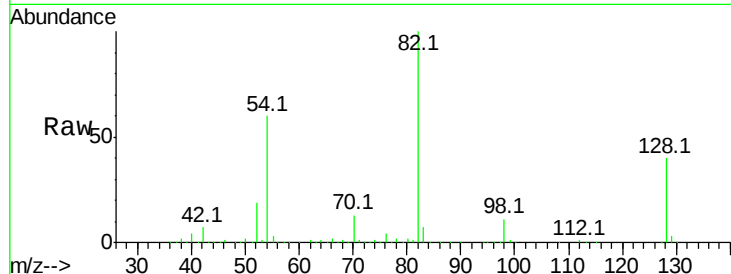


Abundance Ion 82.00 (81.70 to 82.70): BF0
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BF0

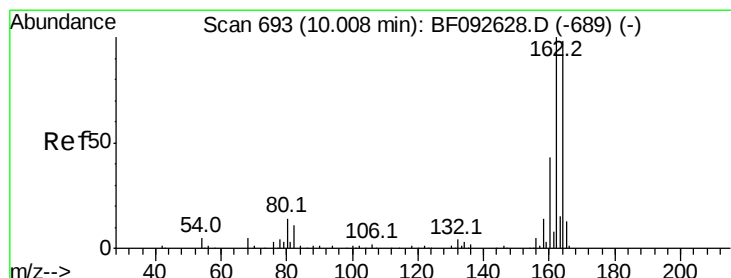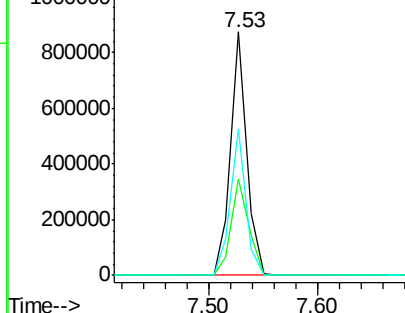
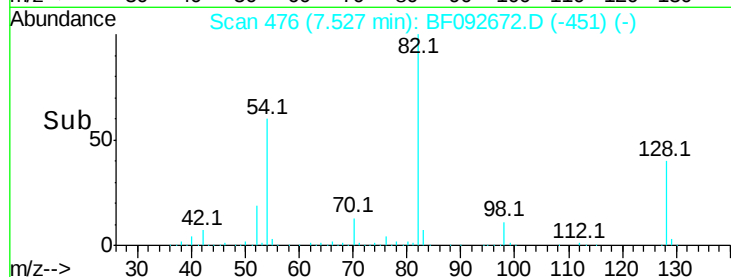



#38
Acenaphthene-d10
Concen: 20.00 ng
RT: 10.01 min Scan# 693
Delta R.T. -0.00 min
Lab File: BF092672.D
Acq: 31 Jan 2017 9:56

Tgt Ion	164	Resp	269629
Ion Ratio <td>100</td> <td>Lower</td> <td>Upper</td>	100	Lower	Upper
162	103.1	80.2	120.2
160	42.8	36.9	55.3

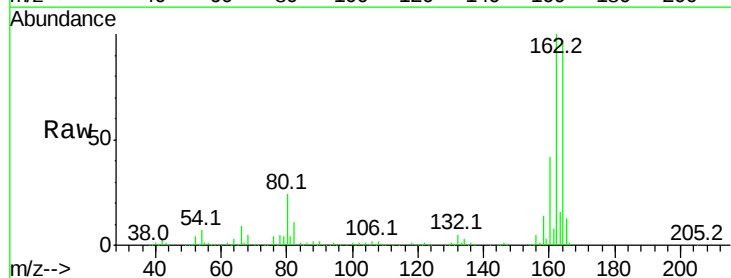

Abundance Ion 164.00 (163.70 to 164.70): E
Ion 162.00 (161.70 to 162.70): E
Ion 160.00 (159.70 to 160.70): E

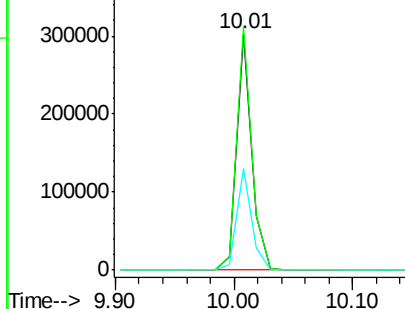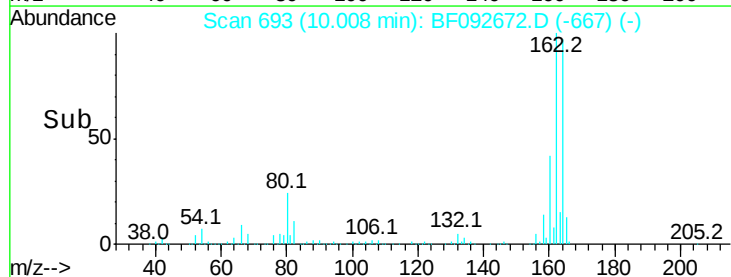


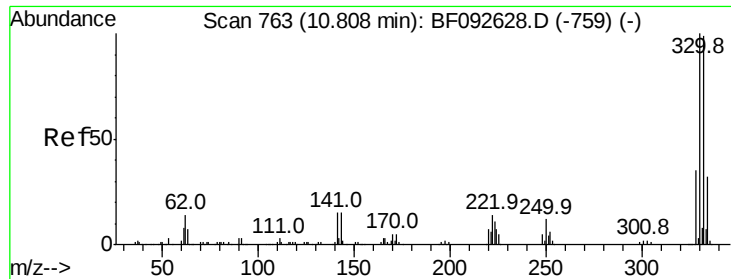




#41
 2,4,6-Tribromophenol
 Concen: 124.69 ng
 RT: 10.81 min Scan# 763
 Delta R.T. -0.00 min
 Lab File: BF092672.D
 Acq: 31 Jan 2017 9:56

Instrument :
 BNA_F
 ClientSampleId :
 W-37

Tot Ion:330 Resp: 243165
 Ion Ratio Lower Upper
 330 100
 332 97.0 77.4 116.2
 141 34.3 34.1 51.1

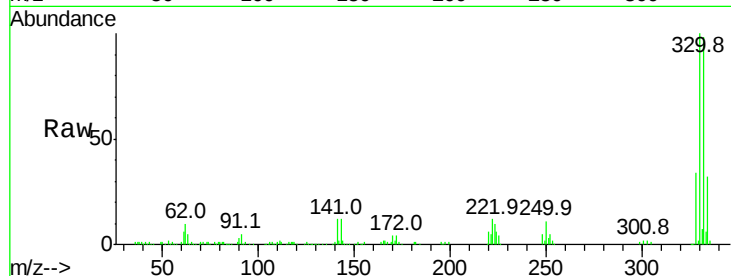


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

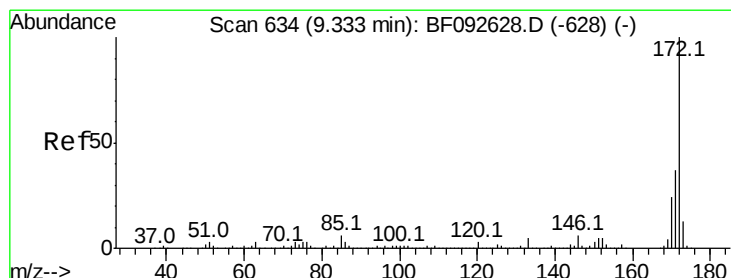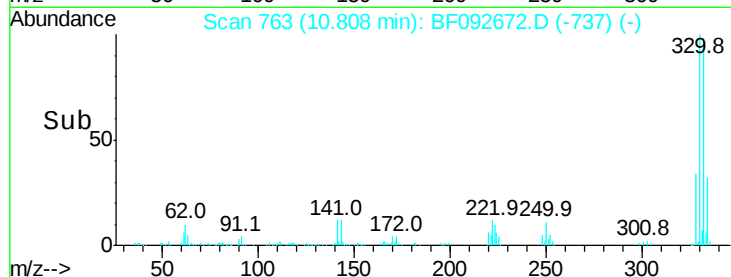
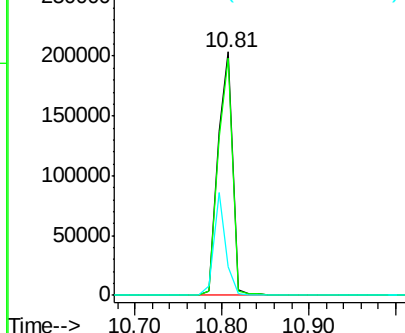



#44
 2-Fluorobiphenyl
 Concen: 104.36 ng
 RT: 9.33 min Scan# 634
 Delta R.T. -0.00 min
 Lab File: BF092672.D
 Acq: 31 Jan 2017 9:56

Tgt Ion:172 Resp: 1553246
 Ion Ratio Lower Upper
 172 100
 171 36.9 29.4 44.0
 170 24.5 20.2 30.4

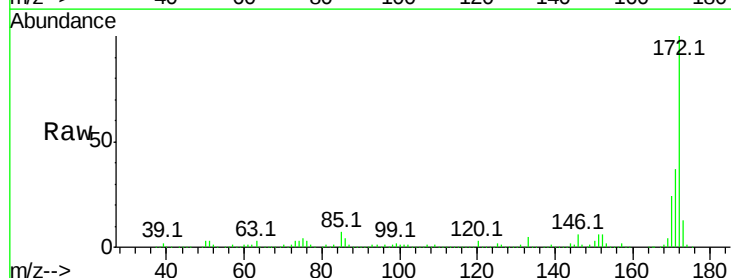

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

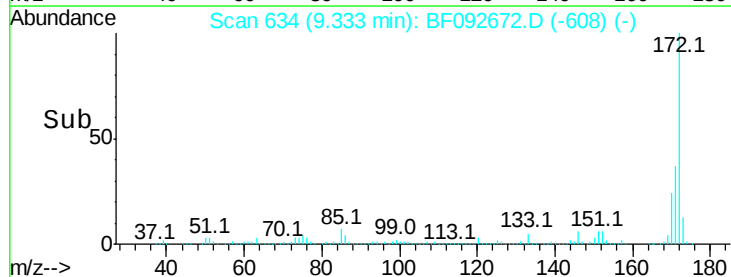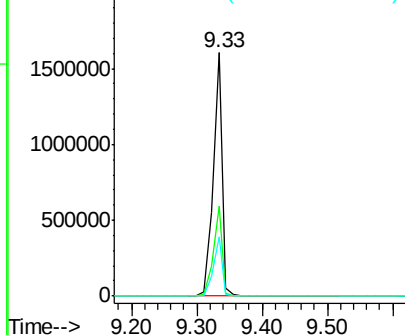


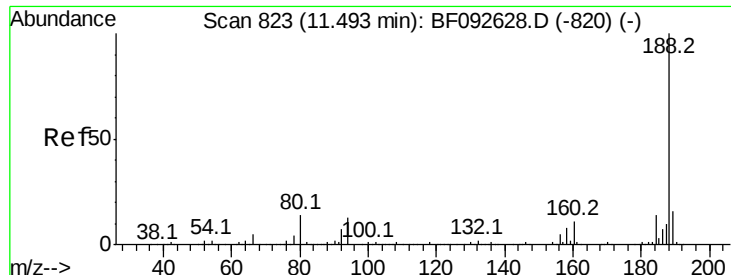




#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 11.49 min Scan# 823
Delta R.T. -0.00 min
Lab File: BF092672.D
Acq: 31 Jan 2017 9:56

Instrument :
BNA_F
ClientSampleId :
W-37

Tot Ion:188 Resp: 372224
Ion Ratio Lower Upper
188 100
94 12.5 10.0 15.0
80 13.1 11.2 16.8

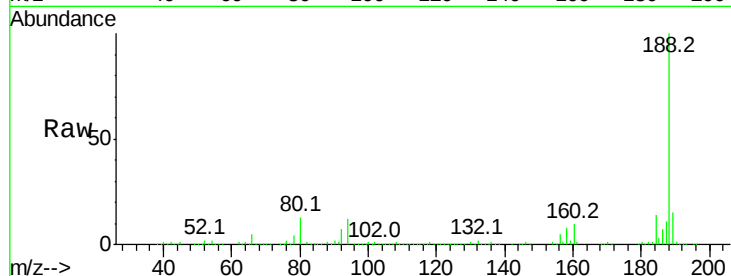


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF0
Ion 80.00 (79.70 to 80.70): BF0

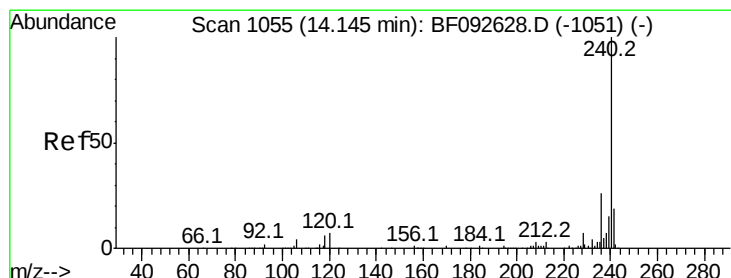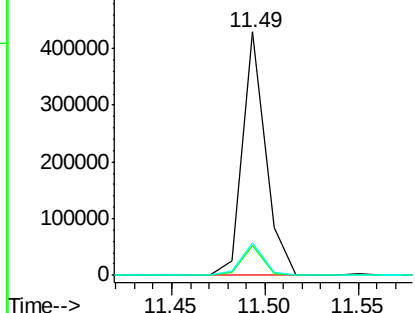
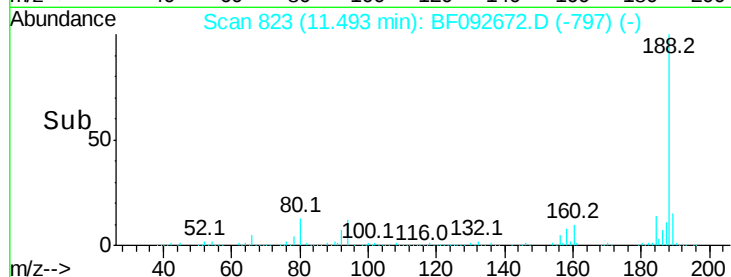



#75
Chrysene-d12
Concen: 20.00 ng
RT: 14.13 min Scan# 1054
Delta R.T. -0.01 min
Lab File: BF092672.D
Acq: 31 Jan 2017 9:56

Tgt Ion:240 Resp: 310154
Ion Ratio Lower Upper
240 100
120 11.7 12.9 19.3#
236 26.0 20.9 31.3

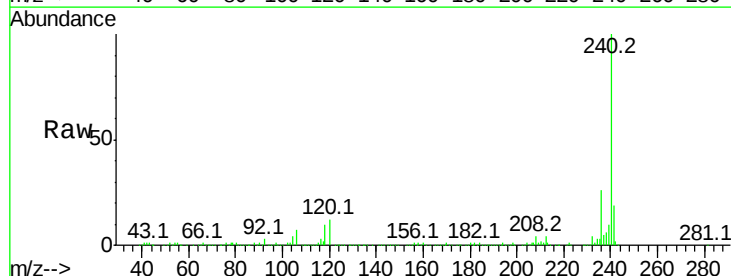

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

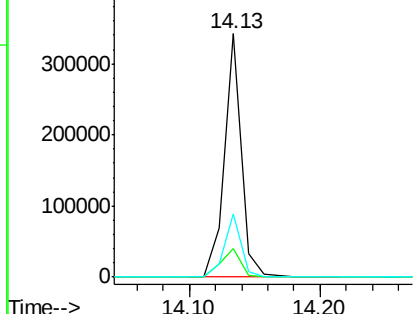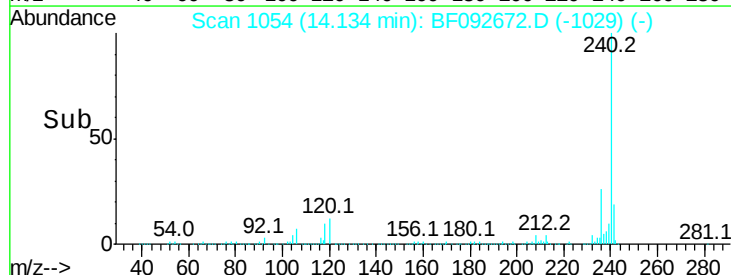


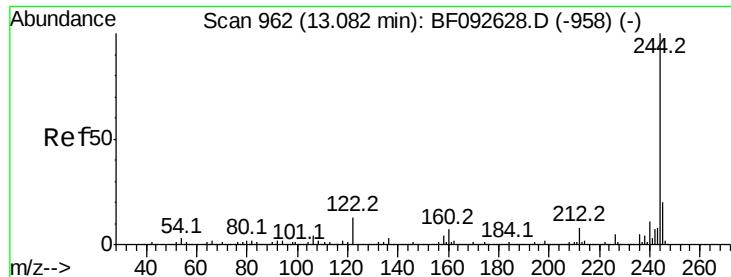




#78
 Terphenyl-d14
 Concen: 79.51 ng
 RT: 13.08 min Scan# 962
 Delta R.T. -0.00 min
 Lab File: BF092672.D
 Acq: 31 Jan 2017 9:56

Instrument :
 BNA_F
 ClientSampleId :
 W-37

Tot Ion:244 Resp: 1049562
 Ion Ratio Lower Upper
 244 100
 212 7.6 6.2 9.2
 122 12.6 11.4 17.2

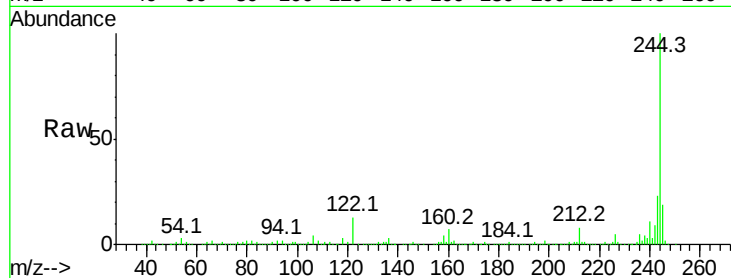


Abundance Ion 244.00 (243.70 to 244.70): E
 Ion 212.00 (211.70 to 212.70): E
 Ion 122.00 (121.70 to 122.70): E

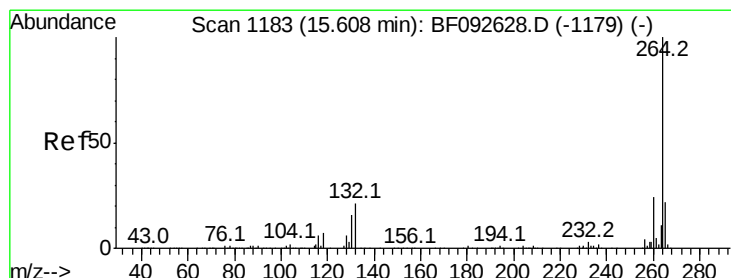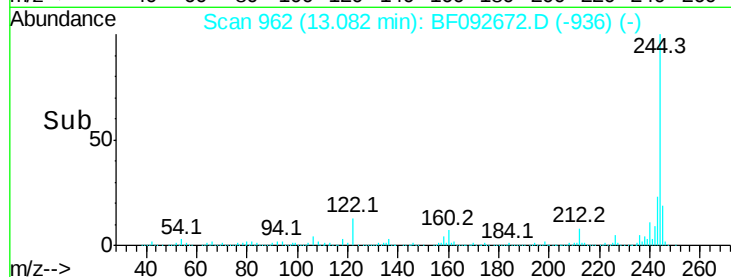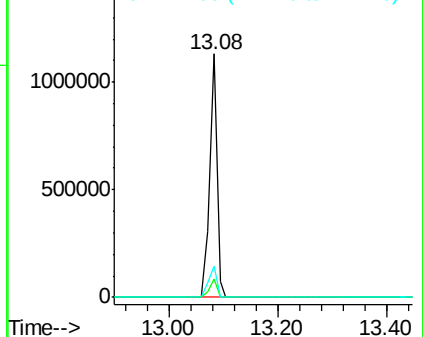

#86
 Perylene-d12
 Concen: 20.00 ng
 RT: 15.61 min Scan# 1183
 Delta R.T. -0.00 min
 Lab File: BF092672.D
 Acq: 31 Jan 2017 9:56

Tgt Ion:264 Resp: 211427
 Ion Ratio Lower Upper
 264 100
 260 23.2 19.2 28.8
 265 21.3 17.4 26.0

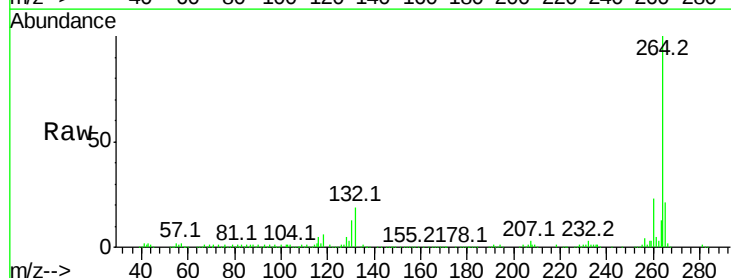

Abundance Ion 264.00 (263.70 to 264.70): E
 Ion 260.00 (259.70 to 260.70): E
 Ion 265.00 (264.70 to 265.70): E

