


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF013017\
 Data File : BF092624.D
 Acq On : 30 Jan 2017 10:12
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF013017.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jan 30 14:50:05 2017

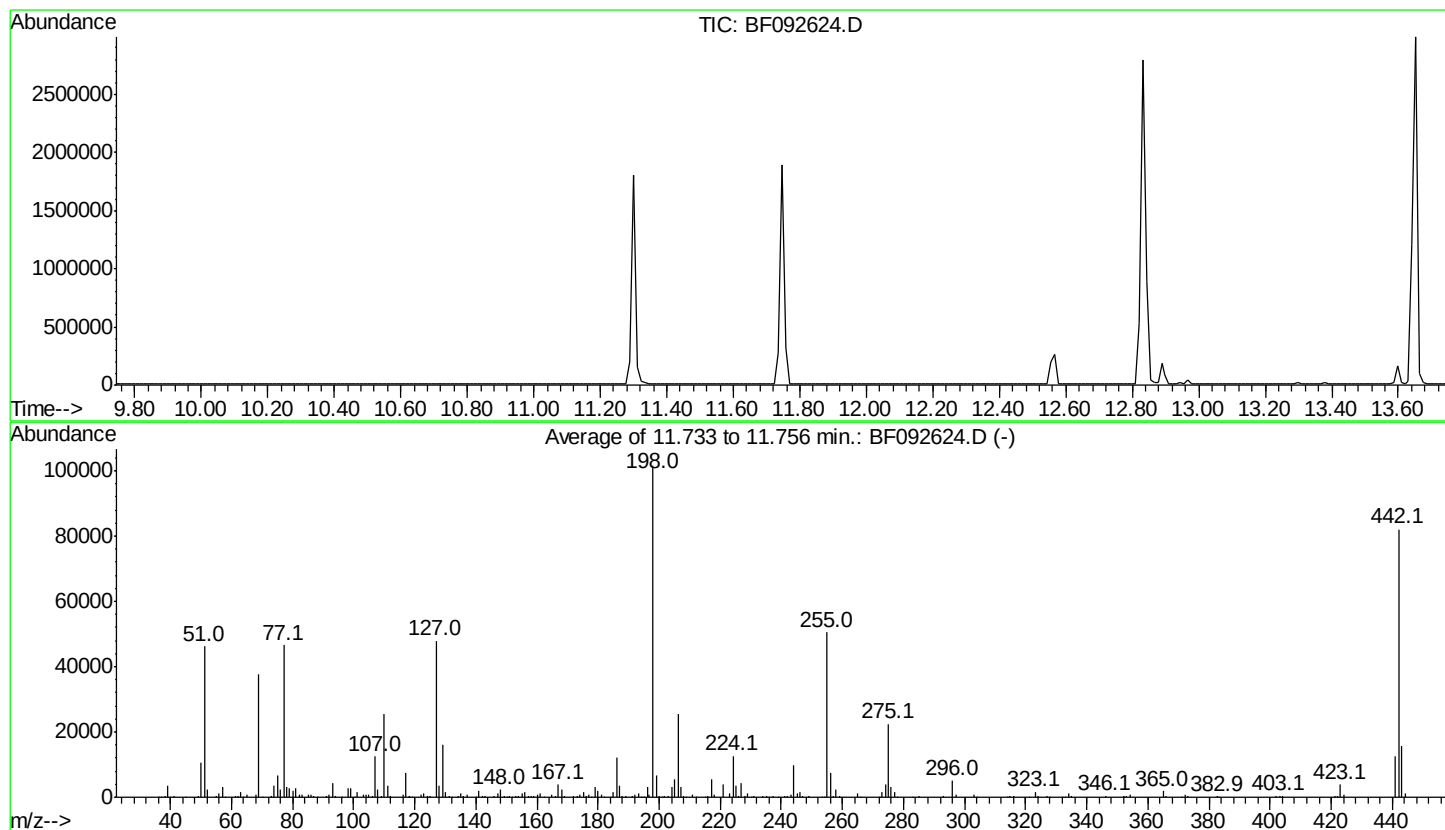

AutoFind: Scans 844, 845, 846; Background Corrected with Scan 841

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.5	46277	PASS
68	69	0.00	2	1.7	644	PASS
69	198	0.00	100	37.0	37591	PASS
70	69	0.00	2	0.4	143	PASS
127	198	10	80	47.2	47956	PASS
197	198	0.00	2	0.9	869	PASS
198	198	100	100	100.0	101602	PASS
199	198	5	9	6.5	6634	PASS
275	198	10	60	22.0	22384	PASS
365	198	1	100	1.9	1935	PASS
441	442	0.01	24	15.5	12689	PASS
442	198	50	100	80.7	82012	PASS
443	442	15	24	19.1	15640	PASS